

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048555.D
 Acq On : 09 Nov 2024 08:04
 Operator : RC/JU
 Sample : P4717-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	28	rBV	37201	47756	0.97%	0.110%
2	3.163	28	30	39	rVB2	20531	27750	0.57%	0.064%
3	3.552	93	96	109	rBV	105104	175737	3.59%	0.404%
4	3.863	145	149	156	rVB	12337	18689	0.38%	0.043%
5	4.228	208	211	217	rVB5	8766	16300	0.33%	0.037%
6	4.369	231	235	244	rBV	44167	71921	1.47%	0.165%
7	4.787	301	306	309	rBV6	4499	8010	0.16%	0.018%
8	5.093	353	358	366	rBV	13386	22985	0.47%	0.053%
9	5.304	391	394	397	rBV5	3371	5734	0.12%	0.013%
10	5.775	470	474	478	rVV3	4688	7810	0.16%	0.018%
11	6.234	547	552	554	rBV6	3491	5273	0.11%	0.012%
12	6.334	563	569	573	rBV8	5361	10085	0.21%	0.023%
13	6.693	627	630	638	rVB5	5328	9790	0.20%	0.022%
14	6.845	650	656	668	rVB	197838	341050	6.96%	0.783%
15	6.998	676	682	694	rBV	603212	957689	19.55%	2.200%
16	7.198	709	716	727	rBV	698151	1129440	23.05%	2.594%
17	7.287	727	731	740	rVB8	8669	18841	0.38%	0.043%
18	7.663	788	795	806	rBV	661995	1062808	21.69%	2.441%
19	8.381	908	917	932	rBV	575428	1017715	20.77%	2.338%
20	8.487	933	935	940	rVB5	5523	7858	0.16%	0.018%
21	8.816	983	991	1007	rBV	664800	1151798	23.51%	2.646%
22	8.951	1010	1014	1024	rVB6	12701	26134	0.53%	0.060%
23	9.539	1106	1114	1125	rBV	575364	966443	19.72%	2.220%
24	10.081	1198	1206	1219	rBV	805942	1472624	30.05%	3.383%
25	10.445	1261	1268	1284	rVB	863712	1497285	30.56%	3.439%
26	10.592	1286	1293	1318	rBV	604881	1228852	25.08%	2.823%
27	12.057	1536	1542	1548	rBV4	9392	19083	0.39%	0.044%
28	13.727	1818	1826	1841	rBV	1472922	2153415	43.95%	4.946%
29	14.004	1863	1873	1885	rBV	1733591	2573686	52.53%	5.912%
30	14.310	1918	1925	1940	rBV	1345014	1909315	38.97%	4.386%
31	14.551	1960	1966	1981	rBV2	67886	198716	4.06%	0.456%
32	15.304	2087	2094	2106	rBV	2108375	3274365	66.83%	7.521%
33	15.439	2111	2117	2130	rVV	606426	903719	18.44%	2.076%
34	15.551	2132	2136	2142	rVB3	12198	19411	0.40%	0.045%
35	15.868	2183	2190	2197	rBV5	10901	21628	0.44%	0.050%
36	16.551	2301	2306	2310	rBV6	11886	21795	0.44%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048555.D
 Acq On : 09 Nov 2024 08:04
 Operator : RC/JU
 Sample : P4717-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.610	2312	2316	2319	rVB5	3789	6071	0.12%	0.014%
38	17.057	2385	2392	2401	rBV	1581097	2178253	44.46%	5.003%
39	17.157	2402	2409	2422	rVV	2614527	3720749	75.94%	8.546%
40	17.462	2456	2461	2464	rVB7	4253	6012	0.12%	0.014%
41	17.727	2502	2506	2509	rBV5	7630	9457	0.19%	0.022%
42	17.957	2542	2545	2552	rBV6	11547	19418	0.40%	0.045%
43	18.386	2614	2618	2622	rBV7	3202	6042	0.12%	0.014%
44	19.015	2721	2725	2730	rBV2	36819	48969	1.00%	0.112%
45	19.086	2733	2737	2742	rVV	32300	46299	0.94%	0.106%
46	19.239	2760	2763	2767	rBV5	11271	16914	0.35%	0.039%
47	19.451	2793	2799	2816	rBV	3247698	4550759	92.87%	10.453%
48	20.950	3050	3054	3063	rVB	154847	212906	4.35%	0.489%
49	21.280	3105	3110	3123	rBV2	1622345	2489597	50.81%	5.718%
50	23.991	3563	3571	3590	rVB	1978787	4899894	100.00%	11.255%
51	24.191	3597	3605	3618	rVB	1165878	2923322	59.66%	6.715%




Sum of corrected areas: 43536172

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048555.D
Acq On : 09 Nov 2024 08:04
Operator : RC/JU
Sample : P4717-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

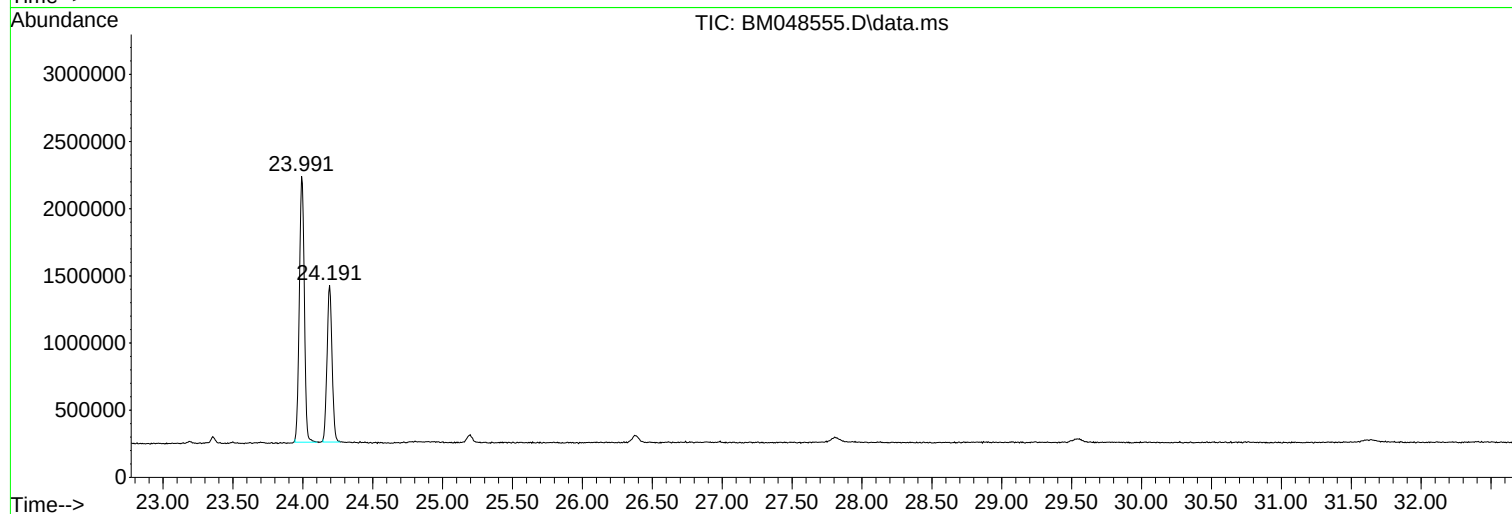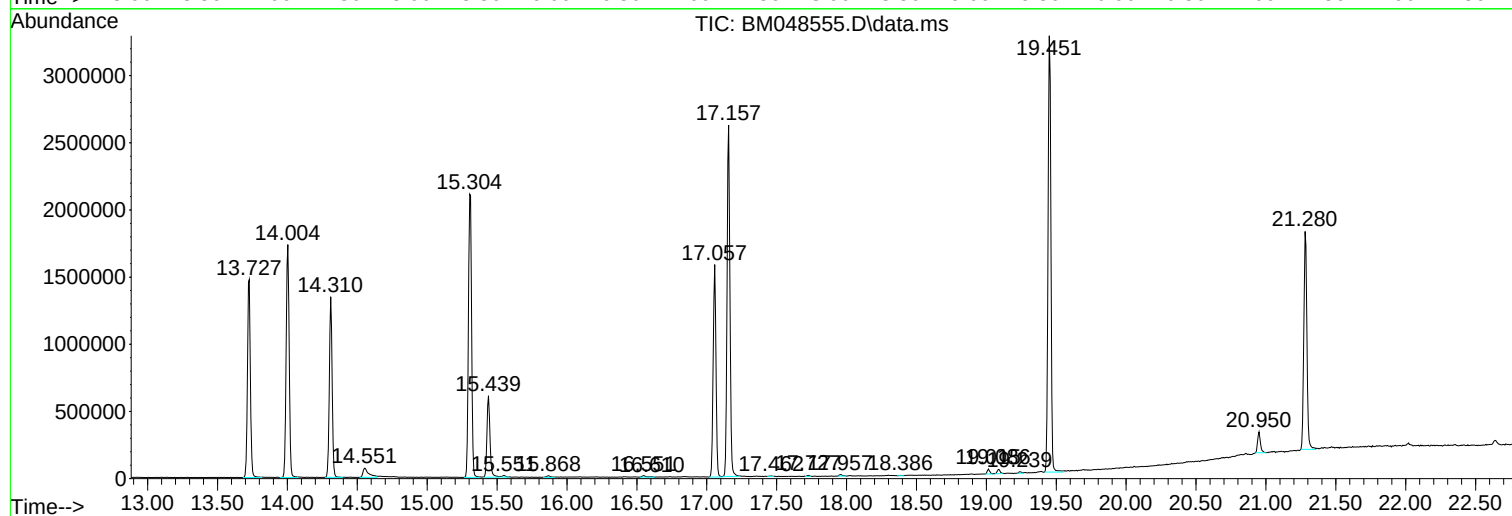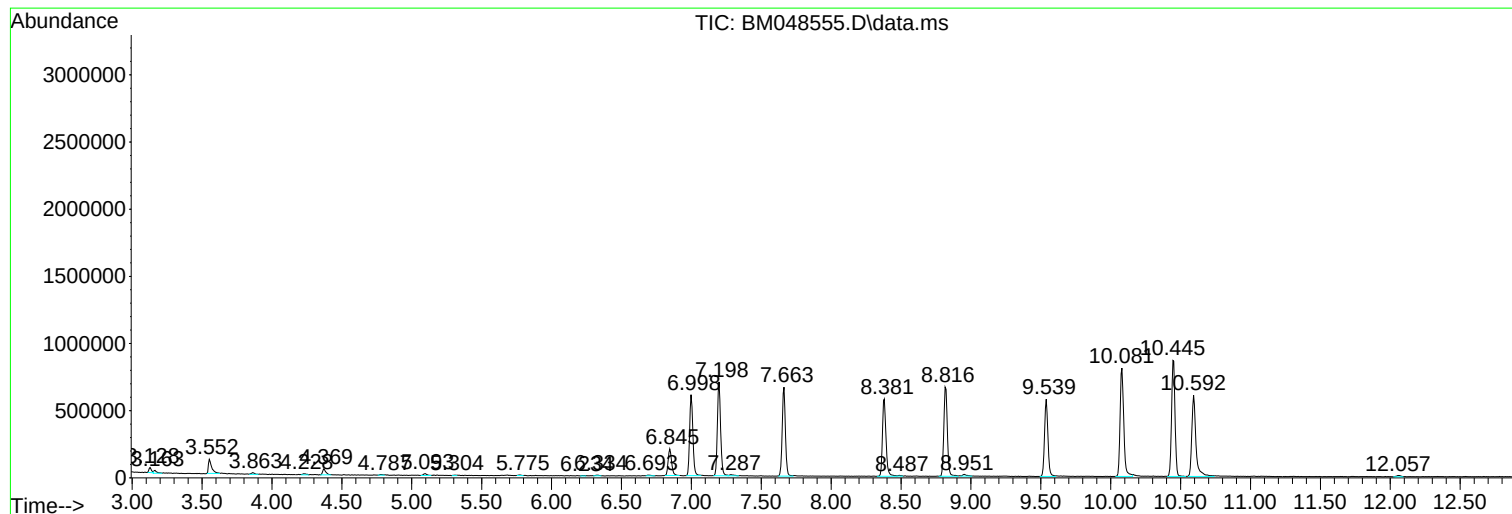

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048555.D
Acq On : 09 Nov 2024 08:04
Operator : RC/JU
Sample : P4717-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048555.D
Acq On : 09 Nov 2024 08:04
Operator : RC/JU
Sample : P4717-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc