

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048557.D
 Acq On : 09 Nov 2024 09:22
 Operator : RC/JU
 Sample : P4717-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	27	rBV	40134	55470	1.11%	0.128%
2	3.157	27	29	33	rVB2	15299	20102	0.40%	0.047%
3	3.546	92	95	110	rBV	140527	248731	4.99%	0.576%
4	3.863	146	149	157	rVB6	12264	18973	0.38%	0.044%
5	4.369	231	235	242	rBV	60619	82356	1.65%	0.191%
6	4.951	330	334	340	rVB7	5566	10891	0.22%	0.025%
7	5.093	355	358	365	rVB2	13655	19829	0.40%	0.046%
8	5.316	390	396	398	rBV6	4771	8608	0.17%	0.020%
9	5.775	470	474	477	rVB5	4269	5459	0.11%	0.013%
10	6.328	561	568	576	rVB10	6036	13675	0.27%	0.032%
11	6.692	627	630	636	rVB7	2949	5800	0.12%	0.013%
12	6.845	646	656	668	rBV	199777	360056	7.22%	0.833%
13	6.998	675	682	695	rBV	627355	1003578	20.13%	2.322%
14	7.198	708	716	726	rBV	706397	1160846	23.29%	2.686%
15	7.663	787	795	803	rBV	615937	1023535	20.53%	2.368%
16	8.381	910	917	930	rBV	565324	989986	19.86%	2.291%
17	8.816	984	991	1009	rBV	677608	1180083	23.67%	2.730%
18	9.245	1062	1064	1069	rVB5	4057	5101	0.10%	0.012%
19	9.539	1106	1114	1134	rBV	574423	990538	19.87%	2.292%
20	10.080	1198	1206	1231	rBV	822305	1514090	30.38%	3.503%
21	10.445	1261	1268	1277	rBV	849766	1439968	28.89%	3.332%
22	10.592	1285	1293	1312	rBV	591472	1220009	24.48%	2.823%
23	12.051	1535	1541	1551	rVB4	10109	23725	0.48%	0.055%
24	12.933	1685	1691	1697	rVB5	4775	10673	0.21%	0.025%
25	13.727	1819	1826	1840	rBV	1464048	2118616	42.50%	4.902%
26	14.004	1865	1873	1881	rBV	1741965	2580459	51.77%	5.971%
27	14.310	1919	1925	1934	rBV	1265240	1813806	36.39%	4.197%
28	14.551	1961	1966	1979	rBV	64613	179037	3.59%	0.414%
29	15.304	2088	2094	2109	rBV	2215791	3224887	64.70%	7.462%
30	15.439	2111	2117	2131	rVV	575736	900334	18.06%	2.083%
31	15.551	2131	2136	2143	rVB4	11923	23543	0.47%	0.054%
32	15.862	2185	2189	2196	rVV4	8068	15477	0.31%	0.036%
33	16.092	2225	2228	2235	rBV6	4132	6275	0.13%	0.015%
34	16.204	2244	2247	2252	rVB6	3950	5574	0.11%	0.013%
35	16.409	2278	2282	2287	rBV5	3251	5312	0.11%	0.012%
36	16.545	2300	2305	2312	rBV8	9446	17094	0.34%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048557.D
Acq On : 09 Nov 2024 09:22
Operator : RC/JU
Sample : P4717-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	16.839	2351	2355	2359	rBV4	3750	5315	0.11%	0.012%
38	17.057	2386	2392	2402	rBV	1520364	2107958	42.29%	4.877%
39	17.157	2402	2409	2422	rVV	2483858	3589873	72.02%	8.306%
40	17.956	2541	2545	2549	rBV5	13835	22405	0.45%	0.052%
41	18.298	2599	2603	2607	rBV7	4294	8256	0.17%	0.019%
42	18.456	2626	2630	2634	rBV7	6047	9964	0.20%	0.023%
43	19.015	2721	2725	2731	rBV3	34354	45871	0.92%	0.106%
44	19.086	2733	2737	2742	rBV	35879	55251	1.11%	0.128%
45	19.239	2759	2763	2768	rBV7	16743	26147	0.52%	0.060%
46	19.303	2772	2774	2777	rBV4	5585	5828	0.12%	0.013%
47	19.450	2793	2799	2811	rBV	3397552	4481444	89.91%	10.369%
48	20.950	3050	3054	3062	rBV	142413	208950	4.19%	0.483%
49	21.280	3105	3110	3121	rBV	1613929	2409645	48.34%	5.575%
50	23.991	3563	3571	3586	rVB	2122968	4984551	100.00%	11.533%
51	24.191	3596	3605	3618	rVB	1176531	2955570	59.29%	6.839%




Sum of corrected areas: 43219524

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048557.D
Acq On : 09 Nov 2024 09:22
Operator : RC/JU
Sample : P4717-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

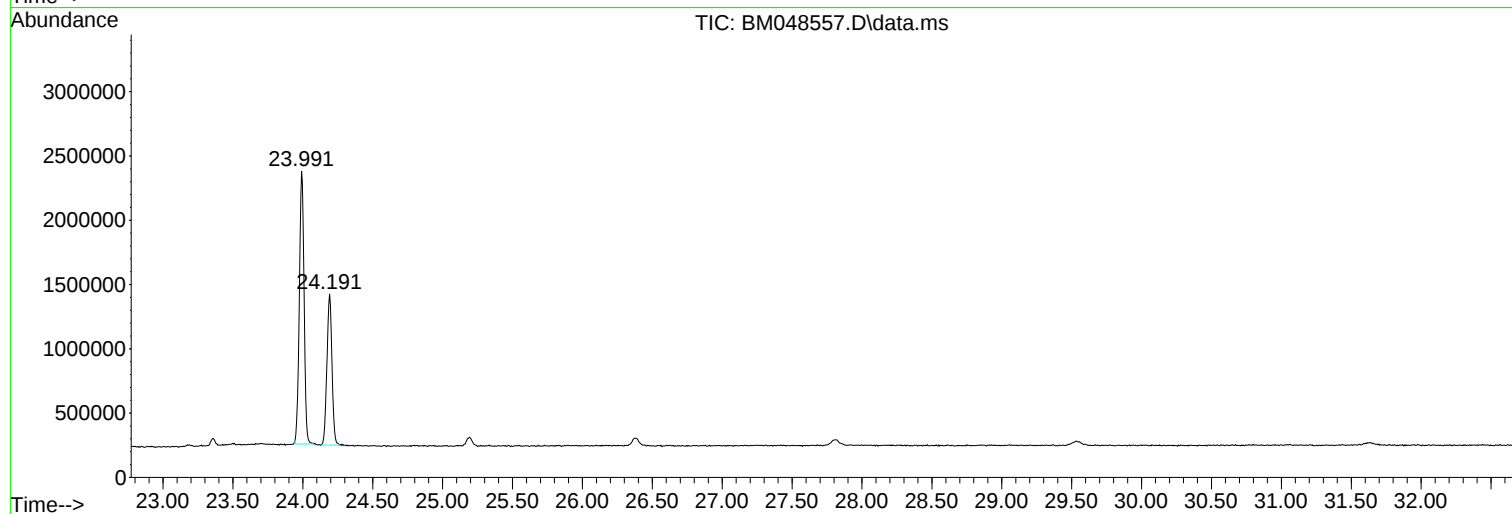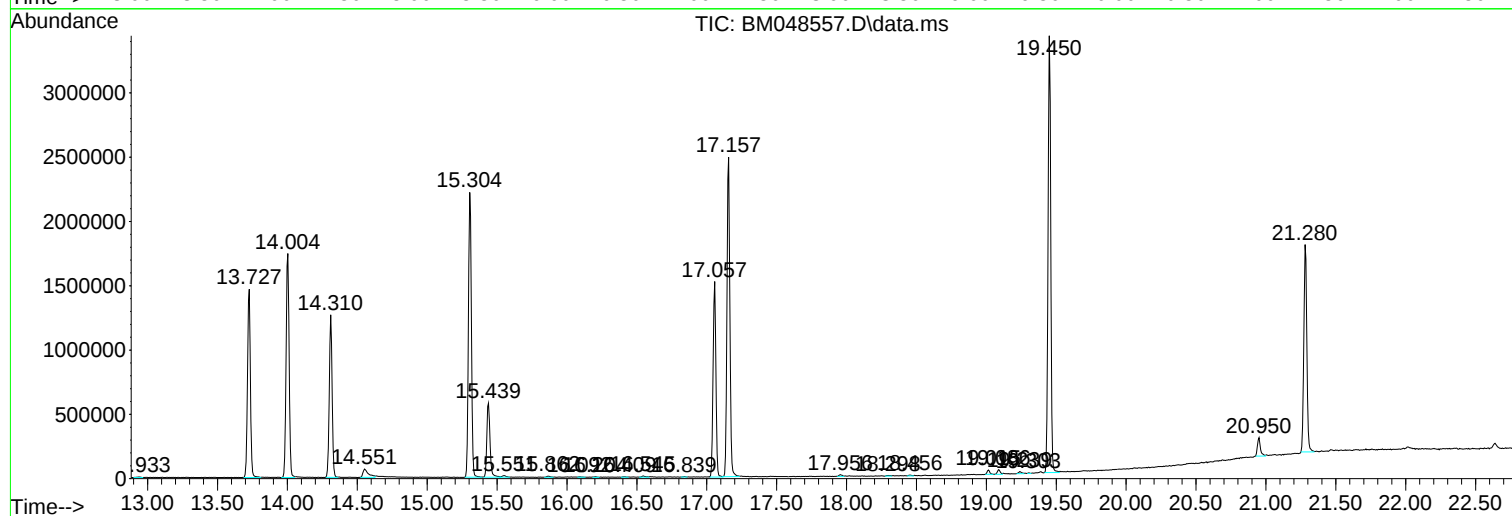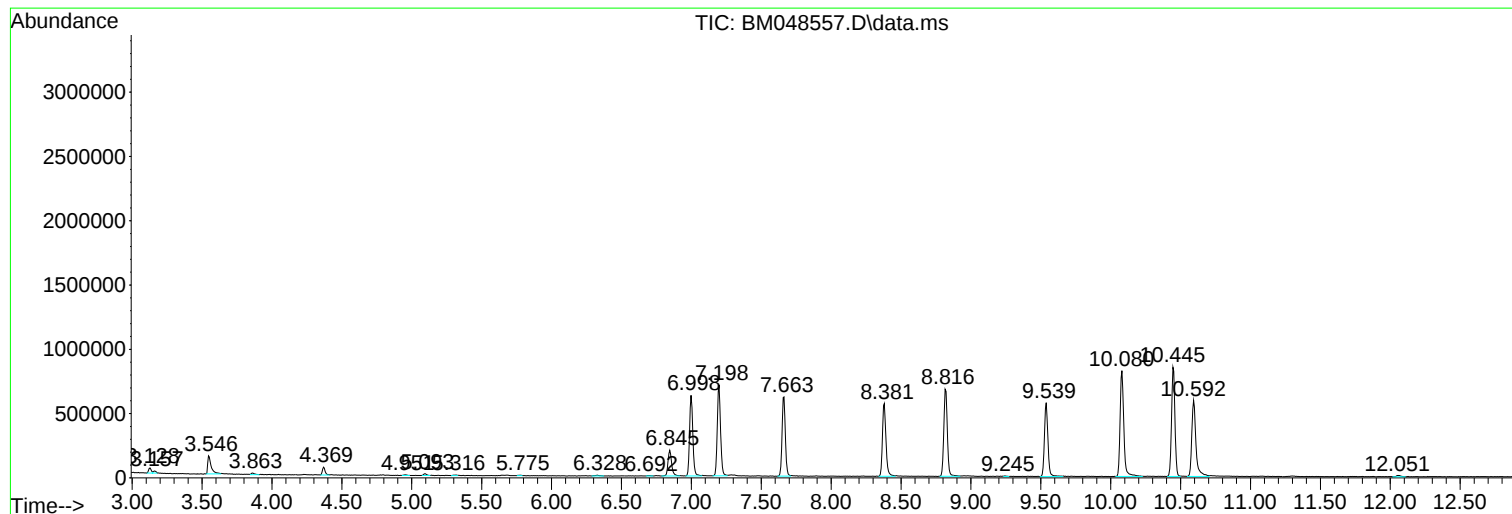

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048557.D
Acq On : 09 Nov 2024 09:22
Operator : RC/JU
Sample : P4717-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048557.D
Acq On : 09 Nov 2024 09:22
Operator : RC/JU
Sample : P4717-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc