

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048564.D
 Acq On : 09 Nov 2024 13:56
 Operator : RC/JU
 Sample : PB164721BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	31	rVB	51959	72542	1.76%	0.160%
2	3.540	90	94	115	rBV	602786	1031458	25.05%	2.271%
3	3.857	145	148	153	rVB4	11168	17077	0.41%	0.038%
4	6.845	648	656	669	rBV	687810	1174445	28.53%	2.586%
5	6.998	676	682	691	rBV	592280	931896	22.64%	2.052%
6	7.198	709	716	727	rBV	765871	1245112	30.24%	2.741%
7	7.663	787	795	802	rBV	744658	1223549	29.72%	2.694%
8	8.375	910	916	930	rBV	842094	1472408	35.77%	3.242%
9	8.816	984	991	1004	rBV	661950	1118385	27.17%	2.462%
10	9.157	1045	1049	1051	rBV3	2940	4373	0.11%	0.010%
11	9.539	1106	1114	1127	rBV	533657	922856	22.42%	2.032%
12	10.081	1198	1206	1227	rBV	801842	1458013	35.42%	3.210%
13	10.445	1261	1268	1280	rBV	1041517	1743074	42.34%	3.838%
14	10.592	1285	1293	1314	rBV	729921	1480416	35.96%	3.260%
15	12.063	1537	1543	1549	rBV3	11985	24462	0.59%	0.054%
16	13.722	1818	1825	1841	rBV	1289796	1926023	46.78%	4.241%
17	14.004	1866	1873	1885	rBV	1596256	2478650	60.21%	5.457%
18	14.310	1918	1925	1937	rBV	1543129	2221178	53.95%	4.891%
19	14.539	1956	1964	1984	rBV	350950	858590	20.86%	1.890%
20	14.986	2037	2040	2044	rVB6	4448	5942	0.14%	0.013%
21	15.304	2088	2094	2103	rBV	2102869	2978244	72.34%	6.557%
22	15.439	2111	2117	2127	rBV	441888	674109	16.37%	1.484%
23	15.551	2130	2136	2142	rVB7	10800	20087	0.49%	0.044%
24	15.863	2183	2189	2195	rBV7	8106	15360	0.37%	0.034%
25	16.410	2277	2282	2287	rBV6	3759	6291	0.15%	0.014%
26	16.551	2300	2306	2311	rBV8	9132	19387	0.47%	0.043%
27	16.845	2350	2356	2360	rBV5	4148	7546	0.18%	0.017%
28	17.057	2385	2392	2402	rBV	1788381	2546293	61.85%	5.606%
29	17.157	2402	2409	2424	rVV	2191824	3188654	77.45%	7.021%
30	17.733	2501	2507	2508	rBV5	3428	4290	0.10%	0.009%
31	17.962	2542	2546	2551	rBV5	5493	10890	0.26%	0.024%
32	18.304	2600	2604	2608	rVB6	4789	7538	0.18%	0.017%
33	19.015	2721	2725	2729	rBV3	31508	41575	1.01%	0.092%
34	19.086	2733	2737	2743	rVV	25976	39544	0.96%	0.087%
35	19.451	2793	2799	2809	rBV	2868647	3844031	93.37%	8.464%
36	20.945	3050	3053	3061	rVB	135818	190276	4.62%	0.419%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048564.D
Acq On : 09 Nov 2024 13:56
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	21.280	3104	3110	3121	rBV	1941737	2907262	70.62%	6.401%
38	23.991	3562	3571	3588	rVB	1652285	4116867	100.00%	9.064%
39	24.191	3596	3605	3619	rVB	1326966	3389349	82.33%	7.463%




Sum of corrected areas: 45418042

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048564.D
Acq On : 09 Nov 2024 13:56
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

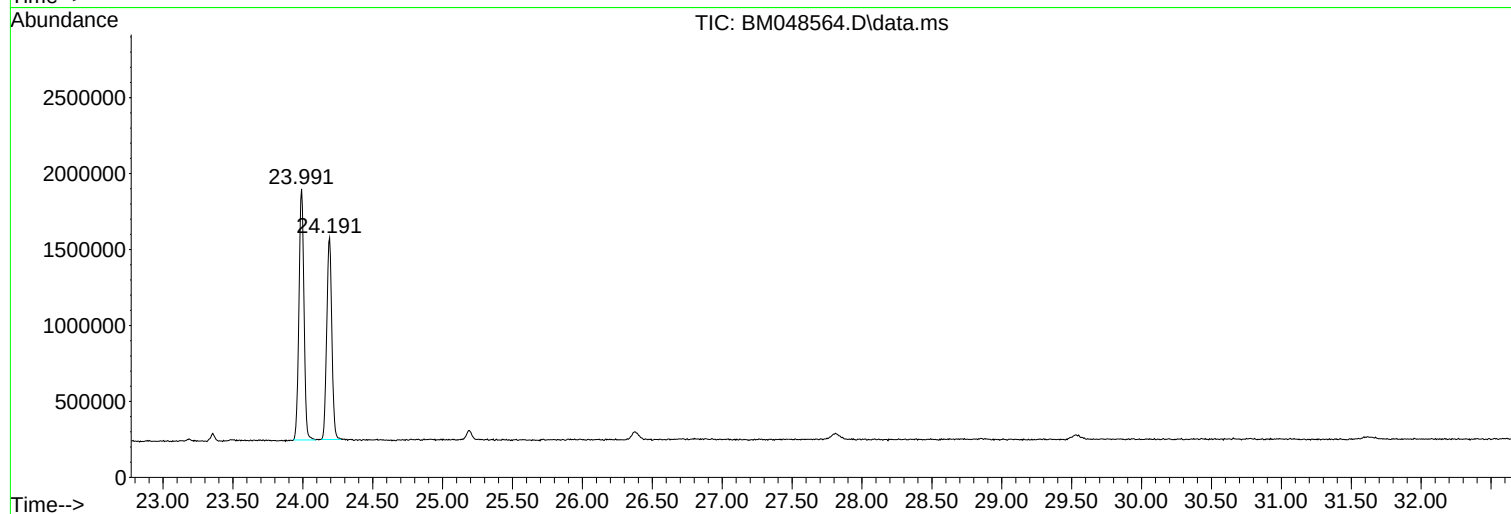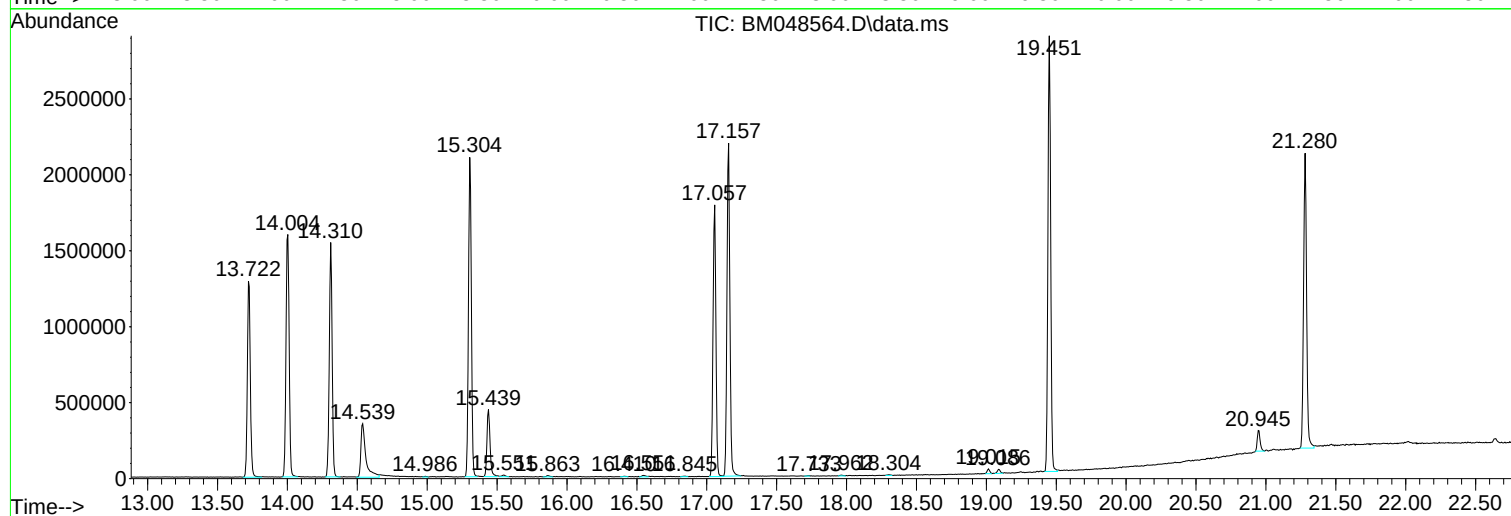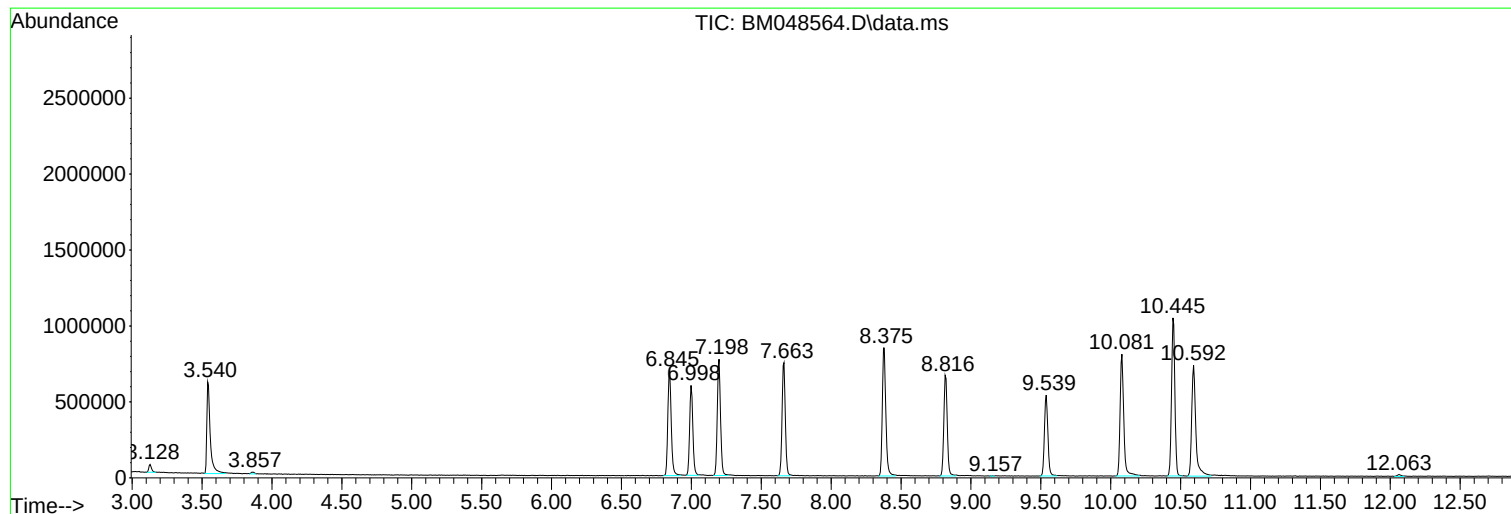

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048564.D
Acq On : 09 Nov 2024 13:56
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048564.D
Acq On : 09 Nov 2024 13:56
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc