

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048566.D
 Acq On : 09 Nov 2024 15:15
 Operator : RC/JU
 Sample : P4627-21
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	35	rVB	38198	62430	1.37%	0.137%
2	3.557	94	97	107	rBV	49386	93782	2.06%	0.206%
3	3.863	144	149	156	rVB	58921	87427	1.92%	0.192%
4	4.781	299	305	311	rVB9	4153	10381	0.23%	0.023%
5	4.957	331	335	339	rVB5	7028	11624	0.26%	0.026%
6	5.640	449	451	455	rBV4	4107	5950	0.13%	0.013%
7	6.845	648	656	666	rBV	148550	288759	6.35%	0.636%
8	6.998	676	682	694	rBV	548906	877899	19.30%	1.932%
9	7.198	709	716	727	rBV	618935	1022524	22.48%	2.251%
10	7.575	777	780	784	rBV5	3205	5057	0.11%	0.011%
11	7.663	787	795	807	rBV	788968	1297722	28.53%	2.857%
12	8.381	910	917	934	rBV	475262	835532	18.37%	1.839%
13	8.816	984	991	1006	rBV	601953	1056543	23.23%	2.326%
14	9.239	1060	1063	1069	rBV7	4692	5572	0.12%	0.012%
15	9.404	1087	1091	1093	rBV5	3586	5854	0.13%	0.013%
16	9.539	1107	1114	1121	rBV	505408	861531	18.94%	1.896%
17	10.081	1199	1206	1227	rBV	732536	1377863	30.30%	3.033%
18	10.445	1261	1268	1284	rVB	1100541	1847692	40.63%	4.067%
19	10.592	1286	1293	1311	rBV	453022	951653	20.93%	2.095%
20	11.275	1403	1409	1413	rBV8	5261	10747	0.24%	0.024%
21	12.057	1534	1542	1551	rBV2	9531	21434	0.47%	0.047%
22	13.139	1721	1726	1732	rVB6	3328	6429	0.14%	0.014%
23	13.274	1747	1749	1755	rVB6	2741	4735	0.10%	0.010%
24	13.721	1819	1825	1836	rBV	1396530	2047133	45.01%	4.506%
25	14.004	1864	1873	1882	rBV	1590332	2384777	52.44%	5.249%
26	14.216	1906	1909	1914	rBV5	3582	4994	0.11%	0.011%
27	14.310	1918	1925	1937	rVV	1649807	2405184	52.89%	5.294%
28	14.445	1944	1948	1954	rVV8	2564	4979	0.11%	0.011%
29	14.557	1961	1967	1986	rBV	58828	195284	4.29%	0.430%
30	14.757	1996	2001	2009	rVB	8466	20369	0.45%	0.045%
31	15.116	2057	2062	2064	rBV3	5581	7987	0.18%	0.018%
32	15.139	2064	2066	2069	rVV	7442	8733	0.19%	0.019%
33	15.168	2069	2071	2077	rVB4	5077	6003	0.13%	0.013%
34	15.304	2087	2094	2101	rBV	2175052	3159164	69.46%	6.954%
35	15.357	2101	2103	2111	rVV5	20991	39434	0.87%	0.087%
36	15.439	2111	2117	2130	rVV	595646	904682	19.89%	1.991%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048566.D
 Acq On : 09 Nov 2024 15:15
 Operator : RC/JU
 Sample : P4627-21
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	15.545	2132	2135	2145	rVB5	12439	24415	0.54%	0.054%
38	15.674	2152	2157	2162	rBV	121120	166529	3.66%	0.367%
39	15.868	2185	2190	2196	rBV9	8878	17747	0.39%	0.039%
40	15.992	2206	2211	2213	rBV5	3789	4632	0.10%	0.010%
41	16.027	2213	2217	2225	rVB8	7567	14650	0.32%	0.032%
42	16.204	2241	2247	2252	rBV3	6771	12426	0.27%	0.027%
43	16.239	2252	2253	2258	rVB5	4543	5369	0.12%	0.012%
44	16.551	2297	2306	2313	rBV4	10757	22530	0.50%	0.050%
45	16.833	2349	2354	2362	rVB7	5074	12591	0.28%	0.028%
46	16.986	2374	2380	2381	rBV6	4863	5566	0.12%	0.012%
47	17.057	2384	2392	2402	rBV	1903826	2755194	60.58%	6.065%
48	17.157	2402	2409	2421	rBV	2568365	3734269	82.11%	8.220%
49	17.351	2438	2442	2447	rVB2	5105	8203	0.18%	0.018%
50	17.427	2449	2455	2460	rBV	21289	41061	0.90%	0.090%
51	17.727	2503	2506	2511	rVB7	6751	9734	0.21%	0.021%
52	17.957	2540	2545	2553	rBV	122038	193881	4.26%	0.427%
53	18.027	2553	2557	2565	rVB	16884	27856	0.61%	0.061%
54	18.251	2592	2595	2599	rBV5	7765	10487	0.23%	0.023%
55	18.298	2601	2603	2609	rVB7	6078	9514	0.21%	0.021%
56	18.451	2626	2629	2632	rBV5	6220	9202	0.20%	0.020%
57	19.015	2720	2725	2729	rBV	39539	50250	1.10%	0.111%
58	19.092	2733	2738	2741	rBV	31161	47651	1.05%	0.105%
59	19.239	2759	2763	2769	rBV2	54326	82773	1.82%	0.182%
60	19.333	2776	2779	2785	rBV	34032	56547	1.24%	0.124%
61	19.451	2793	2799	2808	rBV	3380416	4547880	100.00%	10.011%
62	20.950	3050	3054	3067	rBV2	144398	350820	7.71%	0.772%
63	21.280	3104	3110	3122	rBV	2106180	3106347	68.30%	6.838%
64	22.821	3368	3372	3380	rVB3	114278	207492	4.56%	0.457%
65	23.991	3562	3571	3589	rVB	1841497	4418838	97.16%	9.727%
66	24.191	3596	3605	3618	rVB	1400116	3537242	77.78%	7.786%



Sum of corrected areas: 45429559

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048566.D
Acq On : 09 Nov 2024 15:15
Operator : RC/JU
Sample : P4627-21
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CR0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

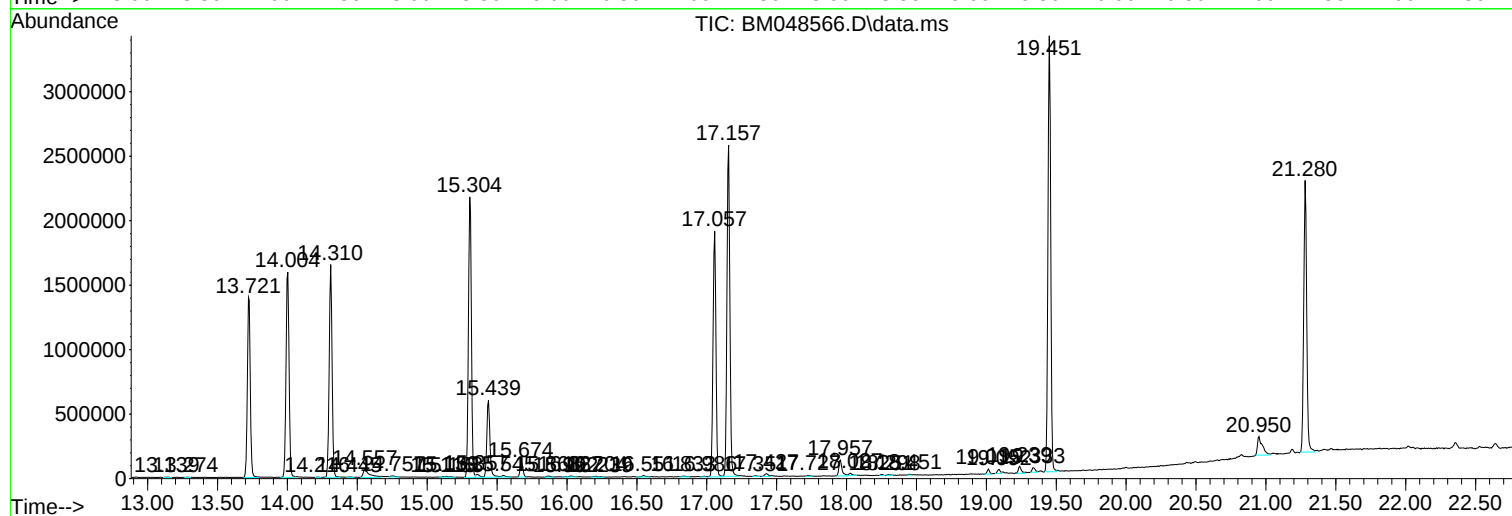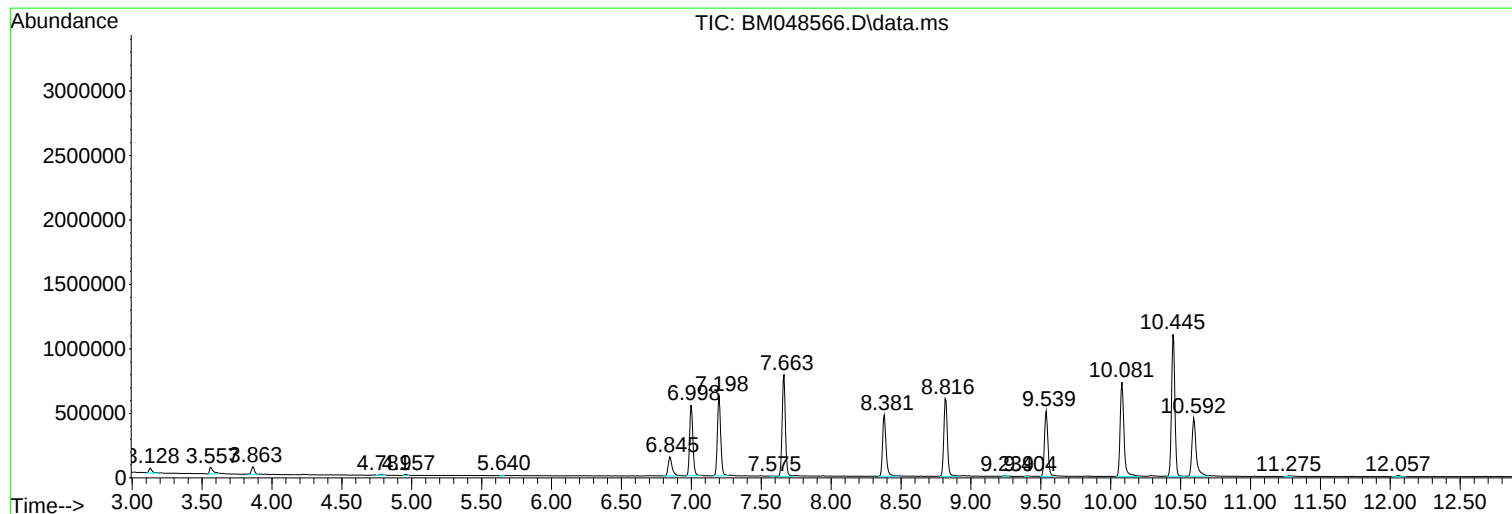

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048566.D
Acq On : 09 Nov 2024 15:15
Operator : RC/JU
Sample : P4627-21
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CR0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048566.D
Acq On : 09 Nov 2024 15:15
Operator : RC/JU
Sample : P4627-21
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CR0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc