

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048567.D
 Acq On : 09 Nov 2024 15:54
 Operator : RC/JU
 Sample : P4644-01
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	21	24	32	rVB	36258	55396	1.06%	0.116%
2	3.552	93	96	111	rBV	173253	331043	6.34%	0.692%
3	3.863	144	149	157	rVB	63042	102687	1.97%	0.215%
4	4.387	232	238	254	rVB	406942	691434	13.24%	1.446%
5	6.846	650	656	672	rBV	182649	350235	6.71%	0.732%
6	6.999	676	682	693	rBV	669833	1058150	20.27%	2.213%
7	7.199	709	716	727	rBV	722323	1193758	22.86%	2.497%
8	7.663	788	795	805	rBV	683220	1122176	21.49%	2.347%
9	8.381	910	917	928	rBV	541314	932115	17.85%	1.949%
10	8.816	984	991	1004	rBV	737239	1263072	24.19%	2.641%
11	8.951	1009	1014	1017	rBV6	4670	7514	0.14%	0.016%
12	9.240	1058	1063	1068	rVB7	4550	8456	0.16%	0.018%
13	9.393	1085	1089	1096	rVB9	6113	12323	0.24%	0.026%
14	9.540	1106	1114	1132	rBV	618379	1056093	20.23%	2.209%
15	10.081	1198	1206	1226	rBV	878894	1611945	30.87%	3.371%
16	10.445	1260	1268	1277	rBV	951387	1595796	30.56%	3.337%
17	10.592	1286	1293	1313	rBV	699703	1442043	27.62%	3.016%
18	10.722	1313	1315	1324	rVB9	4590	11279	0.22%	0.024%
19	11.275	1405	1409	1410	rBV4	3990	6268	0.12%	0.013%
20	12.057	1537	1542	1548	rBV3	9091	18933	0.36%	0.040%
21	12.122	1548	1553	1554	rBV5	5524	7050	0.14%	0.015%
22	13.722	1819	1825	1836	rBV	1605137	2367001	45.34%	4.950%
23	13.998	1865	1872	1891	rBV	1792293	2812700	53.87%	5.882%
24	14.310	1918	1925	1933	rBV	1392285	1994005	38.19%	4.170%
25	14.433	1943	1946	1947	rBV2	5722	5302	0.10%	0.011%
26	14.557	1961	1967	1991	rBV2	62006	210623	4.03%	0.440%
27	14.751	1995	2000	2007	rVB9	7403	18114	0.35%	0.038%
28	15.122	2058	2063	2064	rBV2	5982	8429	0.16%	0.018%
29	15.139	2064	2066	2069	rVV3	7728	9490	0.18%	0.020%
30	15.169	2069	2071	2080	rVB6	5472	8740	0.17%	0.018%
31	15.304	2087	2094	2102	rBV	2466029	3611917	69.18%	7.554%
32	15.439	2110	2117	2131	rBV	638313	987369	18.91%	2.065%
33	15.551	2131	2136	2141	rVB2	13577	21932	0.42%	0.046%
34	15.674	2151	2157	2163	rBV	60134	88066	1.69%	0.184%
35	15.863	2185	2189	2197	rBV5	8167	17178	0.33%	0.036%
36	16.033	2215	2218	2223	rVB6	6344	9139	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048567.D
 Acq On : 09 Nov 2024 15:54
 Operator : RC/JU
 Sample : P4644-01
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CF5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.210	2242	2248	2250	rVB4	5469	7205	0.14%	0.015%
38	16.410	2278	2282	2286	rBV5	4694	7155	0.14%	0.015%
39	16.551	2301	2306	2308	rBV6	12470	19713	0.38%	0.041%
40	16.827	2349	2353	2356	rBV4	3221	5478	0.10%	0.011%
41	16.980	2378	2379	2385	rVB6	4311	5301	0.10%	0.011%
42	17.057	2385	2392	2402	rBV	1598720	2262832	43.34%	4.732%
43	17.157	2402	2409	2420	rBV	2823796	4084148	78.22%	8.541%
44	17.351	2439	2442	2446	rVB3	6687	8367	0.16%	0.017%
45	17.427	2449	2455	2458	rBV	15510	26741	0.51%	0.056%
46	17.733	2499	2507	2511	rBV10	5808	11652	0.22%	0.024%
47	17.951	2540	2544	2550	rBV	86691	129569	2.48%	0.271%
48	18.027	2554	2557	2563	rVB	14882	24525	0.47%	0.051%
49	18.251	2592	2595	2599	rBV6	5726	7079	0.14%	0.015%
50	18.304	2599	2604	2608	rVB7	5749	10708	0.21%	0.022%
51	18.451	2626	2629	2633	rBV6	5267	6704	0.13%	0.014%
52	19.015	2720	2725	2731	rBV2	41389	60583	1.16%	0.127%
53	19.086	2733	2737	2741	rBV	35503	50460	0.97%	0.106%
54	19.239	2759	2763	2770	rBV3	41998	67981	1.30%	0.142%
55	19.339	2776	2780	2785	rBV2	20070	35385	0.68%	0.074%
56	19.386	2786	2788	2792	rVV3	12027	13356	0.26%	0.028%
57	19.451	2793	2799	2812	rVV	3747797	4884811	93.56%	10.216%
58	20.951	3050	3054	3067	rBV	141138	287828	5.51%	0.602%
59	21.280	3105	3110	3122	rBV	1661889	2496076	47.81%	5.220%
60	23.992	3562	3571	3584	rBV	2120673	5221036	100.00%	10.919%
61	24.192	3596	3605	3620	rVB	1204250	3034475	58.12%	6.346%




Sum of corrected areas: 47816939

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048567.D
Acq On : 09 Nov 2024 15:54
Operator : RC/JU
Sample : P4644-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

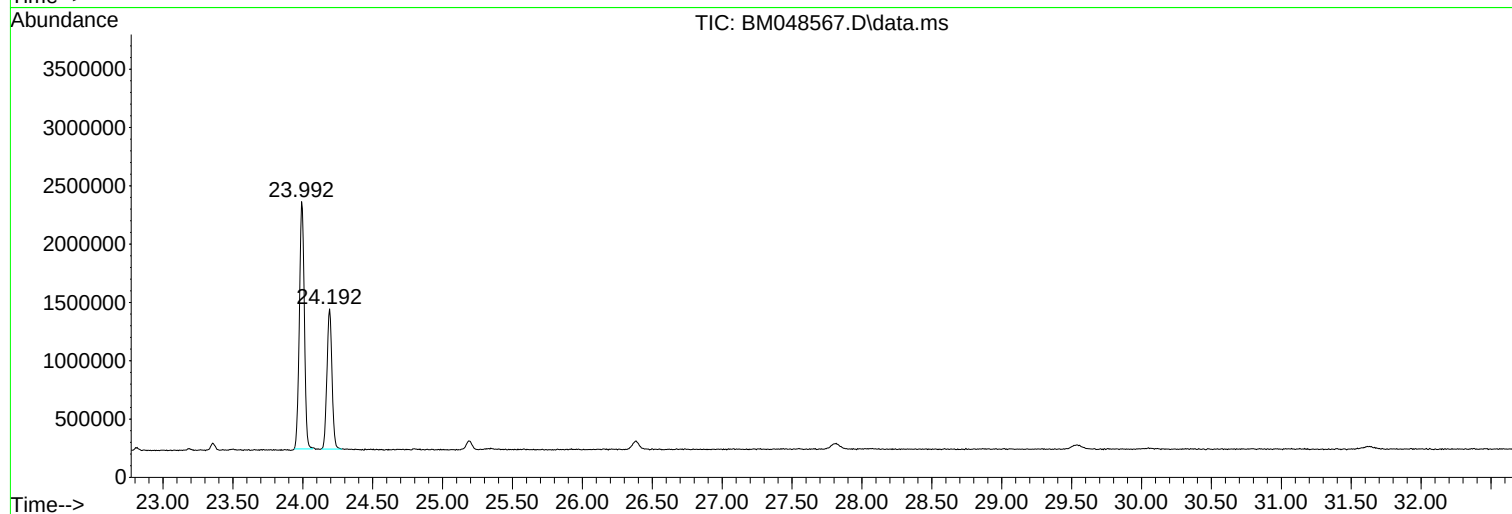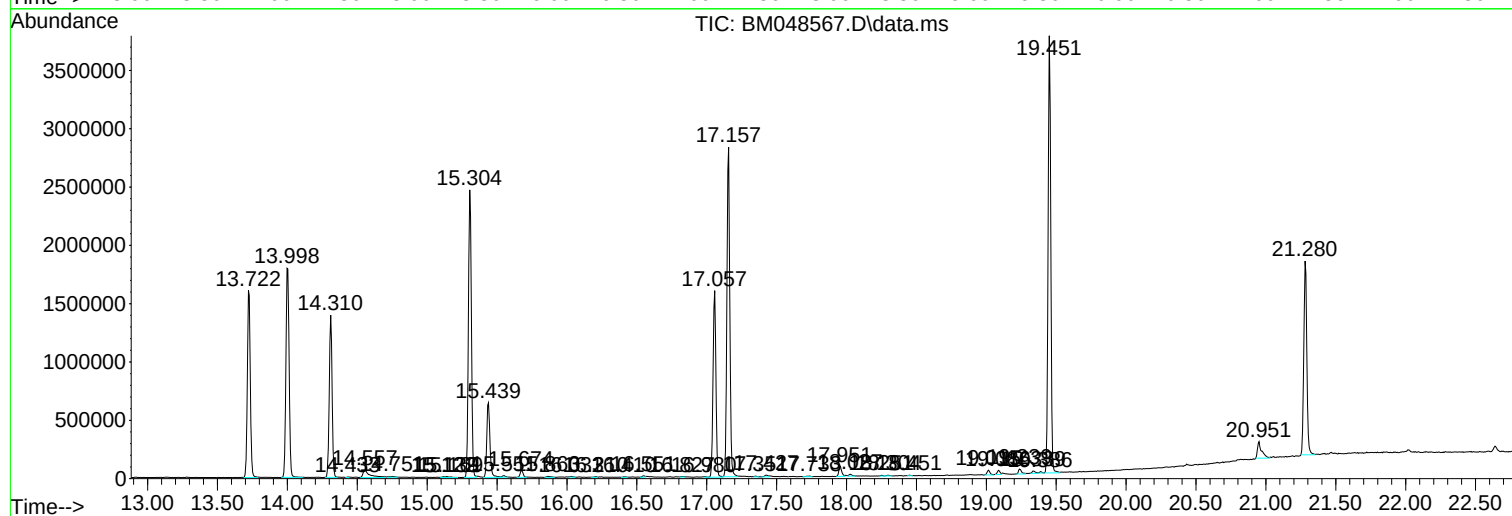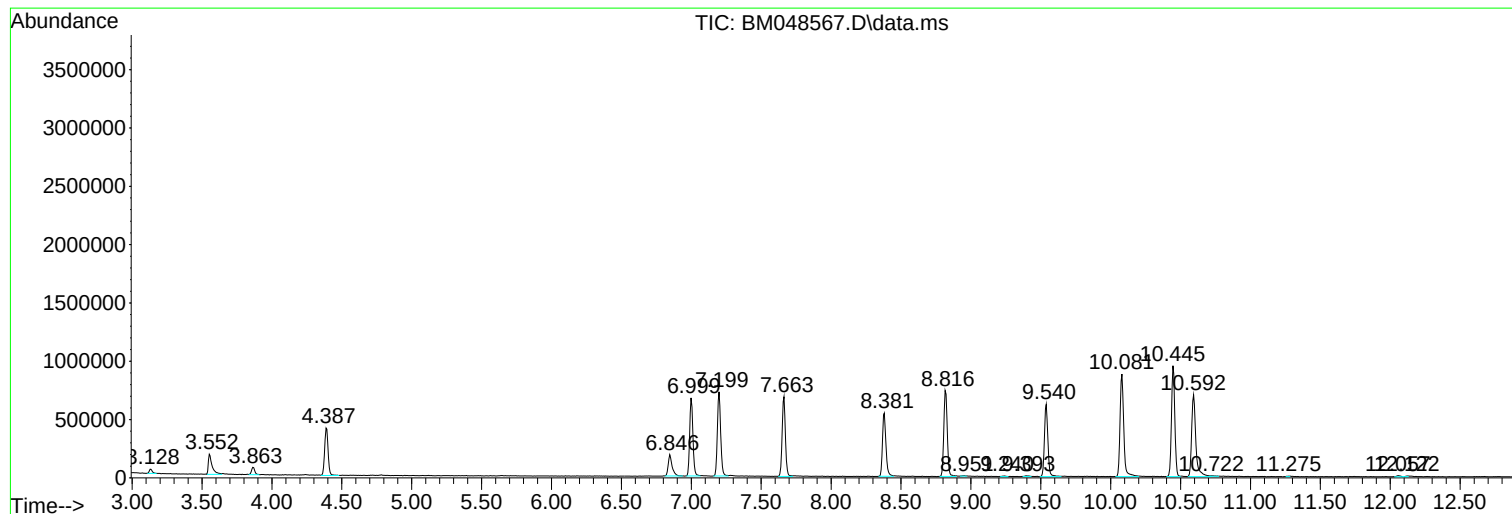

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048567.D
Acq On : 09 Nov 2024 15:54
Operator : RC/JU
Sample : P4644-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF5









Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.387	12.32 ng/ul	691434	1,4-Dichlorobenzene-d4	7.663

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

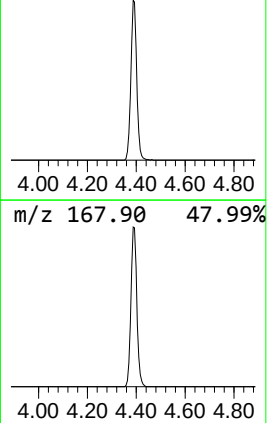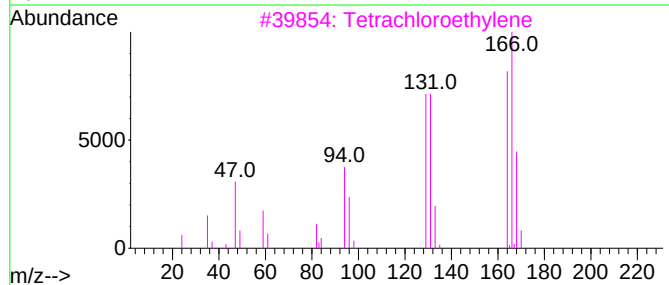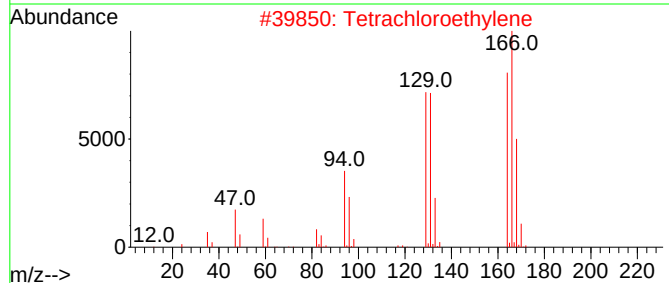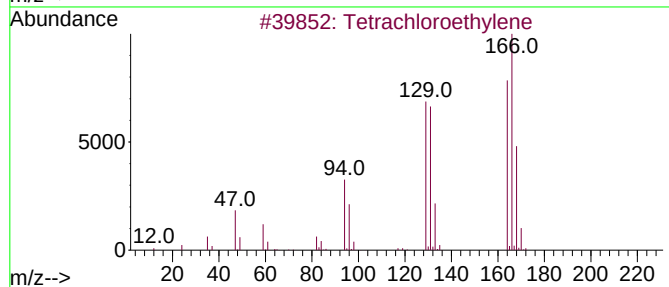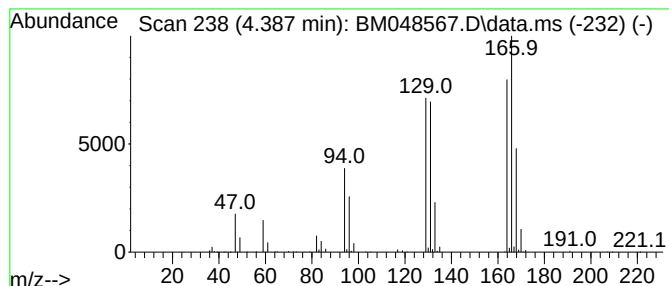

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048567.D
Acq On : 09 Nov 2024 15:54
Operator : RC/JU
Sample : P4644-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.387	12.3	ng/u1	691434	1	7.663	1122180	20.0