

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048570.D
 Acq On : 09 Nov 2024 17:52
 Operator : RC/JU
 Sample : PB164726BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	33	rVB	53499	80105	1.76%	0.159%
2	3.546	91	95	108	rBV	661220	1103158	24.24%	2.194%
3	3.863	147	149	155	rVB3	13236	16865	0.37%	0.034%
4	6.846	649	656	669	rBV	779308	1320466	29.01%	2.626%
5	6.998	676	682	695	rVB	672813	1064388	23.39%	2.116%
6	7.198	709	716	728	rBV	850261	1387579	30.49%	2.759%
7	7.663	788	795	806	rBV	769639	1278386	28.09%	2.542%
8	8.381	910	917	939	rBV	962618	1665633	36.60%	3.312%
9	8.816	984	991	1000	rBV	747440	1258455	27.65%	2.502%
10	9.398	1086	1090	1095	rBV5	1957	4585	0.10%	0.009%
11	9.539	1106	1114	1125	rBV	627205	1058257	23.25%	2.104%
12	10.081	1198	1206	1228	rBV	895760	1671050	36.72%	3.323%
13	10.445	1260	1268	1276	rBV	1096941	1833577	40.29%	3.646%
14	10.592	1286	1293	1313	rBV	767011	1561469	34.31%	3.105%
15	12.063	1537	1543	1549	rBV2	11503	23898	0.53%	0.048%
16	13.722	1818	1825	1833	rBV	1529400	2218751	48.75%	4.412%
17	13.998	1864	1872	1890	rBV	1893878	2889272	63.48%	5.745%
18	14.310	1918	1925	1938	rBV	1632879	2367583	52.02%	4.708%
19	14.533	1957	1963	1985	rBV	449798	1028651	22.60%	2.045%
20	15.304	2087	2094	2103	rBV	2391466	3438151	75.54%	6.836%
21	15.439	2111	2117	2128	rBV	599549	895951	19.69%	1.782%
22	15.545	2132	2135	2141	rVB2	12972	20784	0.46%	0.041%
23	15.863	2185	2189	2193	rBV4	9258	14585	0.32%	0.029%
24	16.092	2222	2228	2230	rBV6	3204	4976	0.11%	0.010%
25	16.204	2244	2247	2251	rVB5	4092	5782	0.13%	0.011%
26	16.545	2302	2305	2308	rBV5	8701	12899	0.28%	0.026%
27	16.739	2335	2338	2344	rVB8	4214	5724	0.13%	0.011%
28	16.839	2351	2355	2359	rBV3	4419	6980	0.15%	0.014%
29	17.057	2385	2392	2402	rBV	1866160	2706089	59.46%	5.381%
30	17.157	2402	2409	2426	rVV	2497017	3738461	82.14%	7.434%
31	17.468	2456	2462	2466	rBV6	4878	8414	0.18%	0.017%
32	17.962	2542	2546	2549	rBV6	5887	8068	0.18%	0.016%
33	18.786	2683	2686	2689	rBV4	3232	5434	0.12%	0.011%
34	19.015	2721	2725	2731	rVB3	34322	45009	0.99%	0.089%
35	19.086	2734	2737	2743	rBV	28758	40696	0.89%	0.081%
36	19.451	2793	2799	2812	rBV	3293348	4401508	96.71%	8.752%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048570.D
Acq On : 09 Nov 2024 17:52
Operator : RC/JU
Sample : PB164726BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK726

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	20.951	3050	3054	3060	rBV	118488	160737	3.53%	0.320%
38	21.280	3104	3110	3122	rBV2	1941007	2969295	65.24%	5.904%
39	23.991	3562	3571	3584	rVB	1894480	4551270	100.00%	9.050%
40	24.186	3596	3604	3620	rVB	1381032	3418632	75.11%	6.798%




Sum of corrected areas: 50291573

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048570.D
Acq On : 09 Nov 2024 17:52
Operator : RC/JU
Sample : PB164726BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

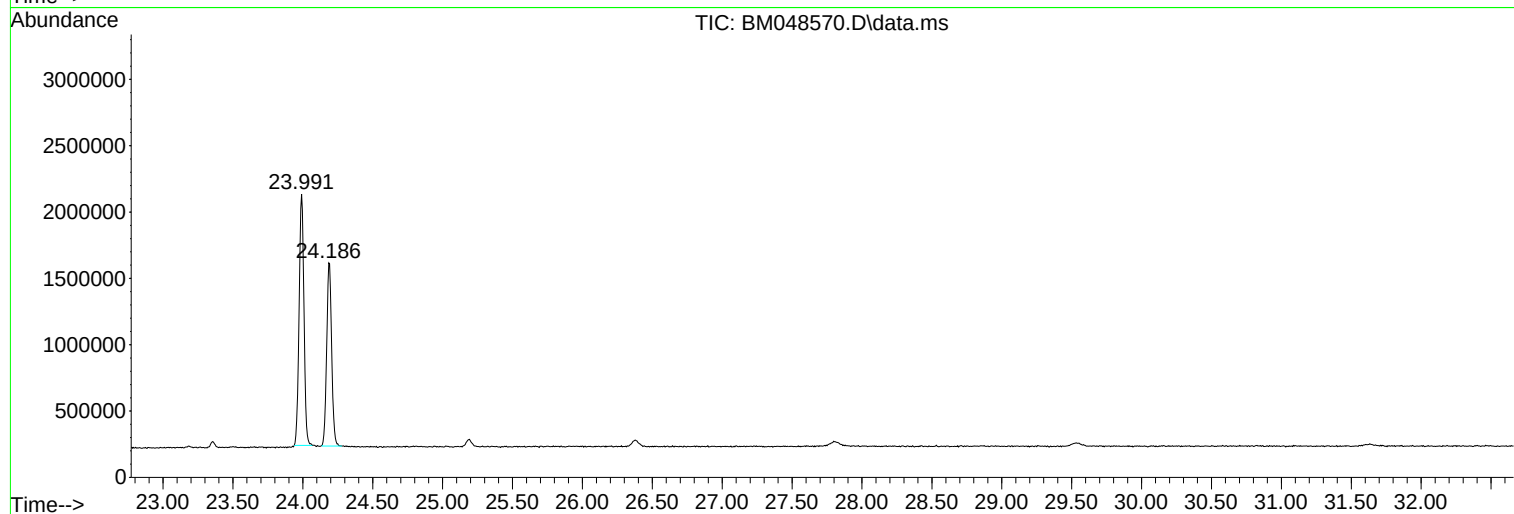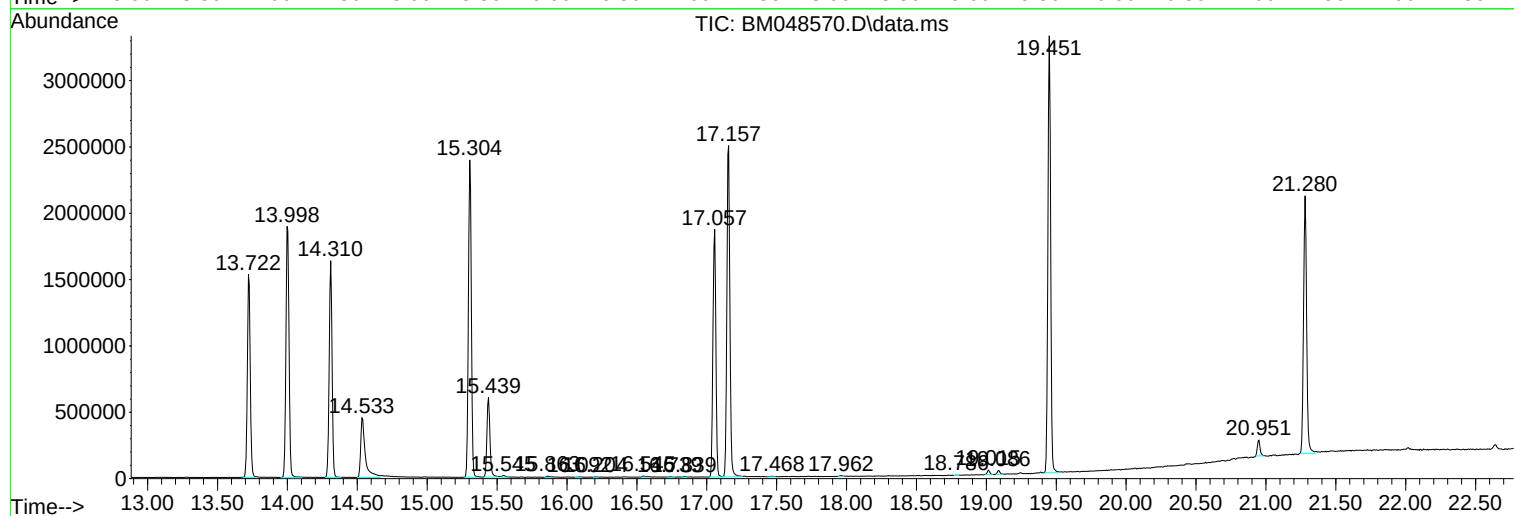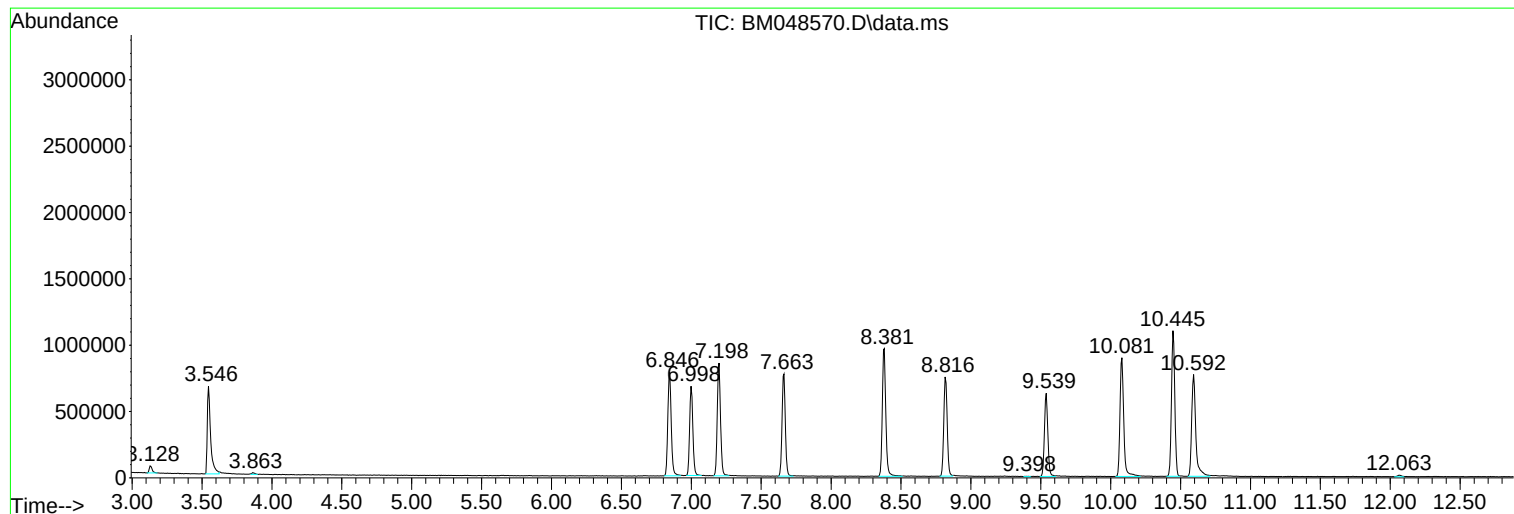

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048570.D
Acq On : 09 Nov 2024 17:52
Operator : RC/JU
Sample : PB164726BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048570.D
Acq On : 09 Nov 2024 17:52
Operator : RC/JU
Sample : PB164726BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc