

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048574.D
 Acq On : 09 Nov 2024 20:29
 Operator : RC/JU
 Sample : P4687-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	30	rVB	40741	53620	1.00%	0.116%
2	3.551	93	96	108	rBV	83784	152829	2.86%	0.331%
3	3.863	145	149	152	rBV	13144	16736	0.31%	0.036%
4	4.369	230	235	241	rBV	58259	81895	1.53%	0.177%
5	5.093	355	358	363	rVB	9703	14283	0.27%	0.031%
6	5.769	468	473	482	rBV3	7632	13114	0.25%	0.028%
7	6.810	645	650	651	rBV5	3993	5534	0.10%	0.012%
8	6.845	651	656	669	rVB	164861	298093	5.58%	0.646%
9	6.998	675	682	697	rBV	602478	972392	18.19%	2.107%
10	7.198	708	716	727	rBV	636013	1081818	20.24%	2.345%
11	7.286	727	731	739	rVB9	7361	17389	0.33%	0.038%
12	7.657	787	794	803	rBV	669510	1111718	20.80%	2.409%
13	8.375	908	916	935	rBV	522834	934015	17.47%	2.024%
14	8.816	984	991	1009	rBV	682012	1165611	21.81%	2.526%
15	9.539	1107	1114	1126	rBV	553300	965719	18.07%	2.093%
16	10.080	1199	1206	1224	rBV	762878	1482064	27.73%	3.212%
17	10.445	1259	1268	1281	rBV	969825	1603061	29.99%	3.474%
18	10.592	1286	1293	1315	rBV	323771	759381	14.21%	1.646%
19	11.080	1375	1376	1383	rVB6	3945	5516	0.10%	0.012%
20	12.063	1537	1543	1548	rBV4	10124	19565	0.37%	0.042%
21	12.927	1689	1690	1699	rVB5	4300	8217	0.15%	0.018%
22	13.721	1819	1825	1839	rBV	1534141	2260327	42.29%	4.899%
23	13.998	1865	1872	1883	rBV	1760201	2645224	49.49%	5.733%
24	14.310	1917	1925	1934	rBV	1463610	2070232	38.73%	4.487%
25	14.551	1961	1966	1981	rBV	63730	189347	3.54%	0.410%
26	15.304	2087	2094	2109	rBV	2387182	3484734	65.20%	7.552%
27	15.439	2111	2117	2129	rVV	688843	1057599	19.79%	2.292%
28	15.551	2131	2136	2141	rVB4	12088	20959	0.39%	0.045%
29	15.674	2152	2157	2165	rBV	73541	102741	1.92%	0.223%
30	15.862	2185	2189	2194	rBV7	8234	14355	0.27%	0.031%
31	16.404	2279	2281	2290	rVB7	3827	8245	0.15%	0.018%
32	16.486	2290	2295	2300	rBV8	2701	5542	0.10%	0.012%
33	16.545	2300	2305	2310	rBV7	11199	19777	0.37%	0.043%
34	17.056	2385	2392	2402	rBV	1675887	2403745	44.97%	5.210%
35	17.151	2402	2408	2422	rBV	2730111	4157816	77.79%	9.011%
36	17.427	2451	2455	2459	rBV	8943	15870	0.30%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
 Data File : BM048574.D
 Acq On : 09 Nov 2024 20:29
 Operator : RC/JU
 Sample : P4687-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CC1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	17.733	2499	2507	2510	rBV9	7401	12831	0.24%	0.028%
38	17.951	2540	2544	2555	rBV2	50266	84136	1.57%	0.182%
39	18.450	2626	2629	2632	rBV5	6927	8994	0.17%	0.019%
40	19.015	2721	2725	2729	rBV2	35760	47897	0.90%	0.104%
41	19.086	2733	2737	2745	rBV	37681	62508	1.17%	0.135%
42	19.239	2759	2763	2769	rBV4	25810	34581	0.65%	0.075%
43	19.345	2777	2781	2783	rBV4	10739	14476	0.27%	0.031%
44	19.386	2786	2788	2792	rVB4	9593	10779	0.20%	0.023%
45	19.450	2793	2799	2812	rVV	3824016	5088650	95.20%	11.028%
46	20.944	3050	3053	3068	rBV	128355	248268	4.64%	0.538%
47	21.280	3104	3110	3126	rBV2	1803870	2804674	52.47%	6.078%
48	23.991	3562	3571	3583	rBV	2252007	5344955	100.00%	11.584%
49	24.191	3596	3605	3619	rVB	1295720	3159415	59.11%	6.847%




Sum of corrected areas: 46141247

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048574.D
Acq On : 09 Nov 2024 20:29
Operator : RC/JU
Sample : P4687-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

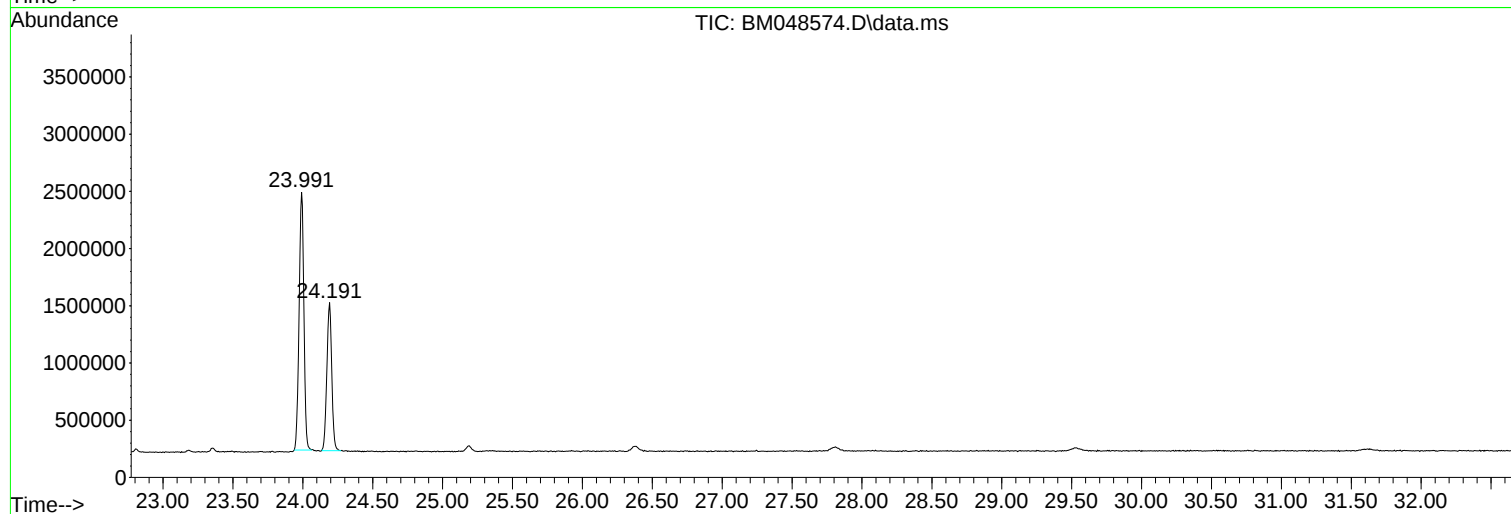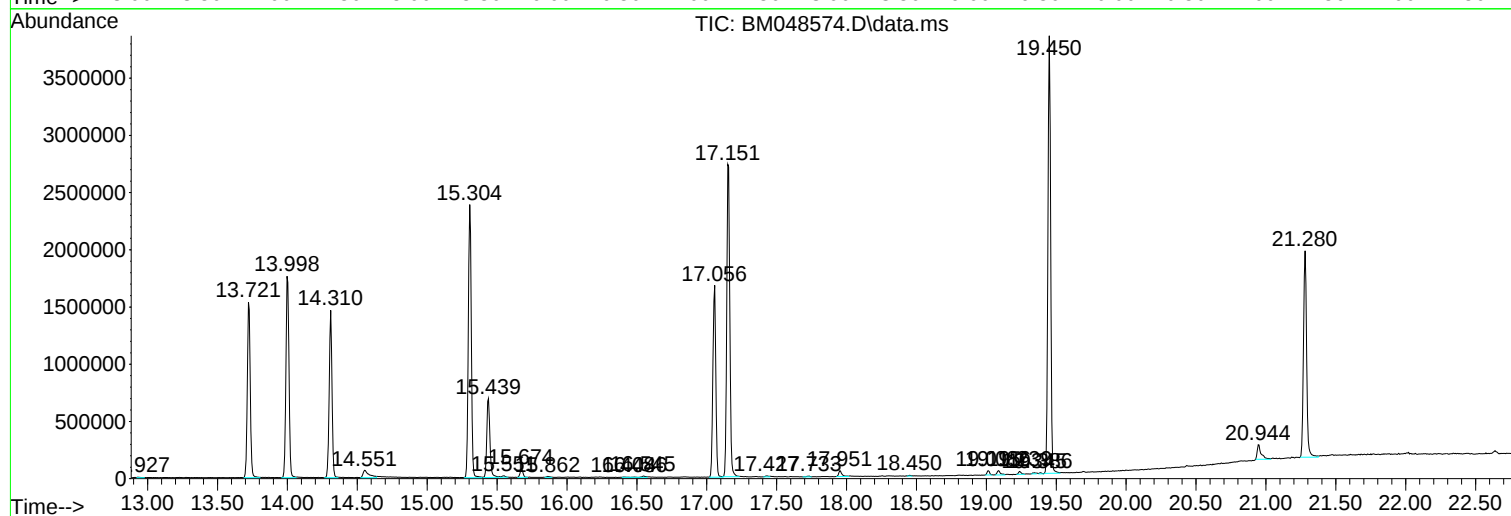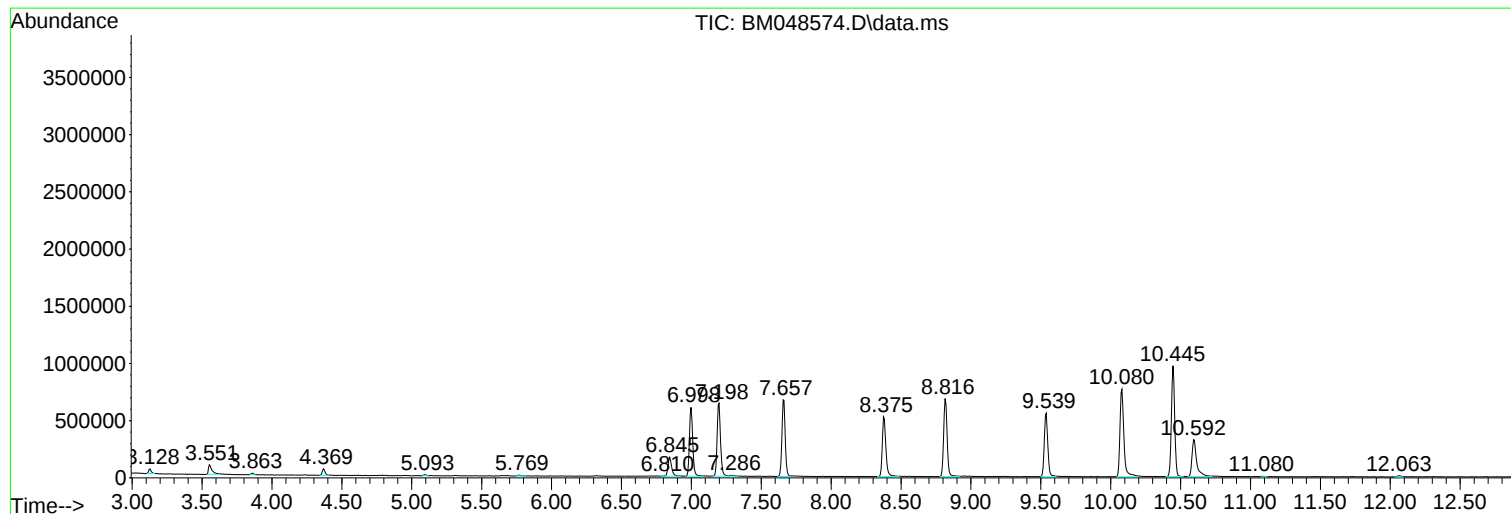

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048574.D
Acq On : 09 Nov 2024 20:29
Operator : RC/JU
Sample : P4687-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110824\
Data File : BM048574.D
Acq On : 09 Nov 2024 20:29
Operator : RC/JU
Sample : P4687-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CC1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc