


Data Path : Z:\HPCHEM1\BNA_M\Data\BM110915\
 Data File : BM003069.D
 Acq On : 09 Nov 2015 14:02
 Operator : UM/IZ
 Sample : DFTPP40
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP40

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 10 02:32:24 2015

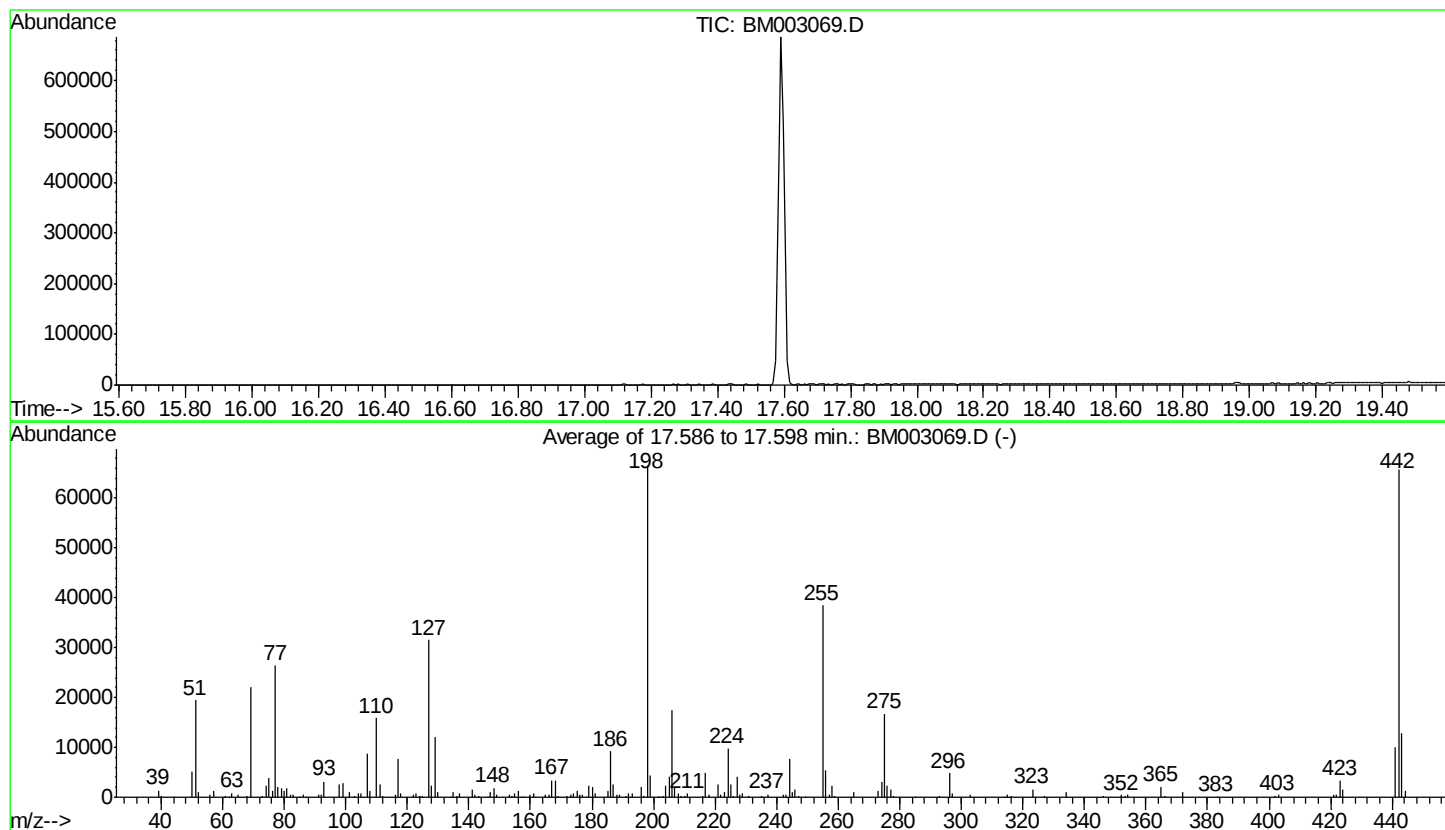

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	19492	PASS
68	69	0.00	2	1.4	311	PASS
69	198	0.00	100	33.3	22149	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	31562	PASS
197	198	0.00	1	0.3	220	PASS
198	198	100	100	100.0	66528	PASS
199	198	5	9	6.6	4371	PASS
275	198	10	60	25.3	16802	PASS
365	198	1	100	3.3	2169	PASS
441	443	0.01	100	78.7	10057	PASS
442	198	50	100	99.0	65840	PASS
443	442	15	24	19.4	12783	PASS

m/z	Abundance
44.00	406.0
207.00	754.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

m/z	Abundance
39.00	1438.0
39.90	329.0
44.00	395.0
50.00	5025.0
51.10	20424.0
52.00	973.0
56.00	579.0
57.00	1328.0
60.90	334.0
63.00	773.0
65.10	437.0
68.00	517.0
69.00	22672.0
73.10	332.0
74.00	2538.0
75.00	4007.0
76.00	1372.0
77.10	26328.0
78.10	2117.0
79.00	1861.0
80.00	1436.0
81.00	1846.0
81.90	426.0
83.00	368.0
86.00	688.0
90.90	476.0
92.00	556.0
93.00	3149.0
98.00	2588.0
99.00	2907.0
101.00	1101.0
103.00	325.0
104.00	762.0
105.00	722.0
107.00	8769.0
108.00	1395.0
110.00	15705.0
111.00	2731.0
116.00	376.0
117.00	7064.0
118.00	744.0
121.90	560.0
123.00	796.0
123.90	431.0
125.00	322.0
127.00	30984.0
128.00	2388.0
129.00	11775.0
130.00	1097.0
134.90	1013.0
136.10	363.0
137.00	909.0
141.00	1519.0
142.00	473.0
147.00	920.0
148.00	1744.0
149.00	604.0
153.00	445.0
154.00	435.0
155.00	723.0
156.00	1210.0
160.00	501.0
161.00	601.0
165.00	558.0
166.10	425.0
167.00	3034.0
168.00	3891.0
169.00	468.0
172.00	346.0
173.00	476.0
174.00	701.0
175.00	1213.0
176.10	459.0
177.00	588.0
179.00	2139.0
180.00	2085.0
181.00	760.0
185.00	1058.0
186.00	8292.0
187.10	2442.0
188.00	439.0
189.00	520.0
191.00	333.0
191.90	685.0
193.00	840.0
196.00	1527.0
196.90	353.0
198.00	60456.0
199.00	4117.0
201.70	312.0
203.10	344.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

204.00	2050.0
205.00	3631.0
206.10	15235.0
207.00	2617.0
208.00	655.0
210.20	325.0
211.00	691.0
216.00	355.0
217.00	4282.0
218.00	532.0
221.00	2242.0
221.80	634.0
223.00	944.0
224.10	8301.0
225.00	2425.0
227.00	3542.0
228.00	432.0
229.00	854.0
237.10	598.0
242.00	435.0
243.10	508.0
244.10	6412.0
245.10	912.0
246.00	1297.0
255.00	32720.0
256.10	4629.0
256.90	483.0
258.00	2013.0
259.00	314.0
265.00	766.0
273.00	956.0
274.00	2533.0
275.10	14225.0
276.00	1991.0
277.10	1102.0
296.00	4004.0
297.10	594.0
303.00	340.0
315.00	346.0
323.10	1149.0
334.10	759.0
352.00	327.0
365.00	1567.0
372.10	644.0
403.10	344.0
421.00	371.0
422.00	335.0
423.10	2356.0
424.10	1300.0
441.10	6764.0
442.10	44648.0
443.10	8875.0
444.10	977.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

m/z	Abundance
39.10	1664.0
44.00	408.0
50.10	6159.0
51.10	23320.0
52.10	1247.0
56.00	732.0
57.00	1524.0
61.00	350.0
62.00	333.0
63.00	998.0
65.00	542.0
68.00	417.0
69.00	26792.0
73.00	386.0
74.00	2778.0
75.00	4788.0
76.10	1493.0
77.10	32056.0
78.00	2320.0
79.00	2046.0
80.00	1570.0
81.00	2454.0
82.00	604.0
83.00	428.0
85.10	322.0
86.00	608.0
86.90	329.0
91.00	557.0
91.90	630.0
93.00	3933.0
98.00	2904.0
99.00	3355.0
101.00	1380.0
103.00	425.0
103.90	901.0
105.00	773.0
107.00	10395.0
108.00	1662.0
110.00	18896.0
111.00	2770.0
111.90	421.0
116.00	618.0
117.00	9424.0
118.00	744.0
122.00	630.0
123.00	1133.0
123.90	490.0
124.90	462.0
127.00	38032.0
128.00	2780.0
129.00	14299.0
130.00	1206.0
134.00	406.0
135.00	1097.0
136.00	550.0
137.00	770.0
141.00	1842.0
142.00	722.0
143.00	486.0
146.00	336.0
147.00	1026.0
148.00	2372.0
149.00	672.0
153.00	574.0
154.00	573.0
155.00	1074.0
156.00	1638.0
157.10	301.0
157.90	374.0
160.00	549.0
161.00	984.0
164.90	707.0
166.00	725.0
167.00	3962.0
168.00	3563.0
169.00	473.0
171.90	320.0
173.00	486.0
174.00	772.0
175.00	1572.0
176.10	370.0
176.90	689.0
178.00	314.0
179.00	2931.0
180.00	2419.0
181.00	875.0
185.10	1524.0
186.10	11060.0
187.00	3065.0
188.00	467.0
189.00	718.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

191.00	491.0
192.00	910.0
193.00	1101.0
196.00	2537.0
196.90	309.0
198.00	79712.0
199.00	5180.0
199.90	384.0
201.30	372.0
203.00	526.0
204.10	3002.0
205.00	5016.0
206.10	21024.0
207.00	3435.0
208.00	807.0
209.00	396.0
210.10	314.0
211.10	818.0
216.10	415.0
217.00	5627.0
218.00	809.0
221.00	3100.0
221.90	670.0
223.00	1304.0
224.10	11839.0
225.00	2921.0
226.00	402.0
227.00	4811.0
228.00	830.0
229.00	979.0
231.10	464.0
235.00	431.0
237.00	718.0
242.00	635.0
243.10	671.0
244.10	8988.0
245.10	1075.0
246.00	1854.0
246.90	321.0
249.10	320.0
255.10	46120.0
256.00	6479.0
257.00	627.0
258.00	2741.0
259.10	454.0
265.00	1134.0
273.00	1412.0
274.00	3644.0
275.10	20008.0
276.10	2724.0
277.00	2030.0
278.00	399.0
285.10	351.0
293.00	450.0
296.00	5928.0
297.00	811.0
303.00	812.0
314.10	331.0
315.00	642.0
316.00	468.0
323.10	1940.0
327.00	351.0
334.00	1274.0
346.10	424.0
352.00	506.0
353.10	407.0
354.00	659.0
365.00	2643.0
366.00	341.0
372.00	1077.0
383.10	307.0
402.00	414.0
403.10	686.0
421.10	726.0
422.00	619.0
423.10	3987.0
424.10	1795.0
441.10	12062.0
442.10	77496.0
443.10	15284.0
444.10	1330.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

m/z	Abundance
39.10	1063.0
39.90	320.0
44.00	593.0
50.00	4131.0
51.10	14732.0
52.00	807.0
56.00	444.0
57.00	1067.0
63.00	785.0
65.00	372.0
69.00	16984.0
74.00	1721.0
75.00	2823.0
76.00	1116.0
77.10	20880.0
78.00	1533.0
79.00	1338.0
80.00	1079.0
81.00	1429.0
81.90	352.0
83.00	438.0
86.00	486.0
91.10	364.0
92.00	398.0
93.00	2351.0
98.00	1881.0
99.00	1880.0
101.00	798.0
102.90	349.0
104.00	546.0
105.00	545.0
107.00	7234.0
108.00	1139.0
110.00	12979.0
111.00	1939.0
116.00	371.0
117.00	6333.0
118.00	562.0
122.00	425.0
123.00	644.0
125.00	339.0
127.00	25672.0
128.00	1814.0
129.00	9969.0
130.00	800.0
134.90	897.0
137.10	709.0
140.90	1345.0
142.00	418.0
143.00	332.0
147.00	843.0
148.00	1579.0
149.00	427.0
153.00	421.0
155.00	809.0
156.10	1124.0
159.90	345.0
161.00	611.0
165.10	585.0
166.00	412.0
167.00	3211.0
168.00	2575.0
173.00	300.0
174.10	571.0
175.00	1236.0
176.00	374.0
176.90	548.0
179.00	2028.0
180.00	1902.0
181.00	641.0
185.00	1080.0
186.00	8066.0
187.00	2395.0
188.00	330.0
189.00	439.0
190.90	332.0
191.90	648.0
193.10	773.0
196.00	1803.0
198.00	59416.0
199.00	3818.0
204.00	2145.0
205.10	3699.0
206.10	15793.0
207.00	2592.0
208.00	727.0
208.90	315.0
210.90	726.0
216.00	321.0
217.00	4616.0
218.00	529.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

221.00	2496.0
221.90	541.0
223.00	895.0
224.10	9043.0
225.10	2209.0
226.10	310.0
227.00	3667.0
228.00	524.0
229.00	890.0
230.90	303.0
237.00	545.0
242.00	541.0
243.00	484.0
244.10	7429.0
245.10	1014.0
246.00	1388.0
247.00	322.0
255.10	36464.0
256.10	5244.0
257.00	507.0
258.00	2028.0
258.90	359.0
264.90	850.0
273.00	1146.0
274.00	2795.0
275.10	16173.0
276.10	2362.0
277.00	1545.0
277.90	372.0
293.00	389.0
296.10	4560.0
297.00	617.0
303.00	609.0
315.00	520.0
323.10	1590.0
324.00	317.0
326.90	304.0
334.10	1066.0
352.00	472.0
353.00	318.0
354.10	659.0
365.00	2298.0
366.10	376.0
372.10	1035.0
402.10	385.0
403.00	448.0
421.00	550.0
422.00	509.0
423.10	3635.0
424.10	1318.0
441.10	11346.0
442.10	75376.0
443.10	14192.0
444.10	1294.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40