

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110916\
 Data File : BM007792.D
 Acq On : 09 Nov 2016 12:12
 Operator : UM/SJ
 Sample : H5575-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBBM5

Quant Time: Nov 09 16:37:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 16:26:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	177316	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	691140	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	451707	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.13	188	916995	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	1178763	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1222253	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	5356	1.29	ng/uL	0.00
5) Phenol-d5	6.92	99	91199	6.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	230803	28.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	252402	24.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	162784	15.20	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	146749	29.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	161905	30.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	275267	26.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	128	0.01	ng/ul	0.02
43) Dimethylphthalate-d6	13.79	166	951067	30.92	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	1125643	30.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	22808	4.69	ng/ul	0.02
57) Fluorene-d10	15.37	176	825335	30.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	132936	24.40	ng/ul	0.00
70) Anthracene-d10	17.22	188	1305755	31.60	ng/ul	0.00
76) Pyrene-d10	19.52	212	1548991	31.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1676052	31.41	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
64) N-Nitrosodiphenylamine	15.64	169	27883	1.06	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110916\
Data File : BM007792.D
Acq On : 09 Nov 2016 12:12
Operator : UM/SJ
Sample : H5575-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBBM5

Quant Time: Nov 09 16:37:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 16:26:14 2016
Response via : Initial Calibration

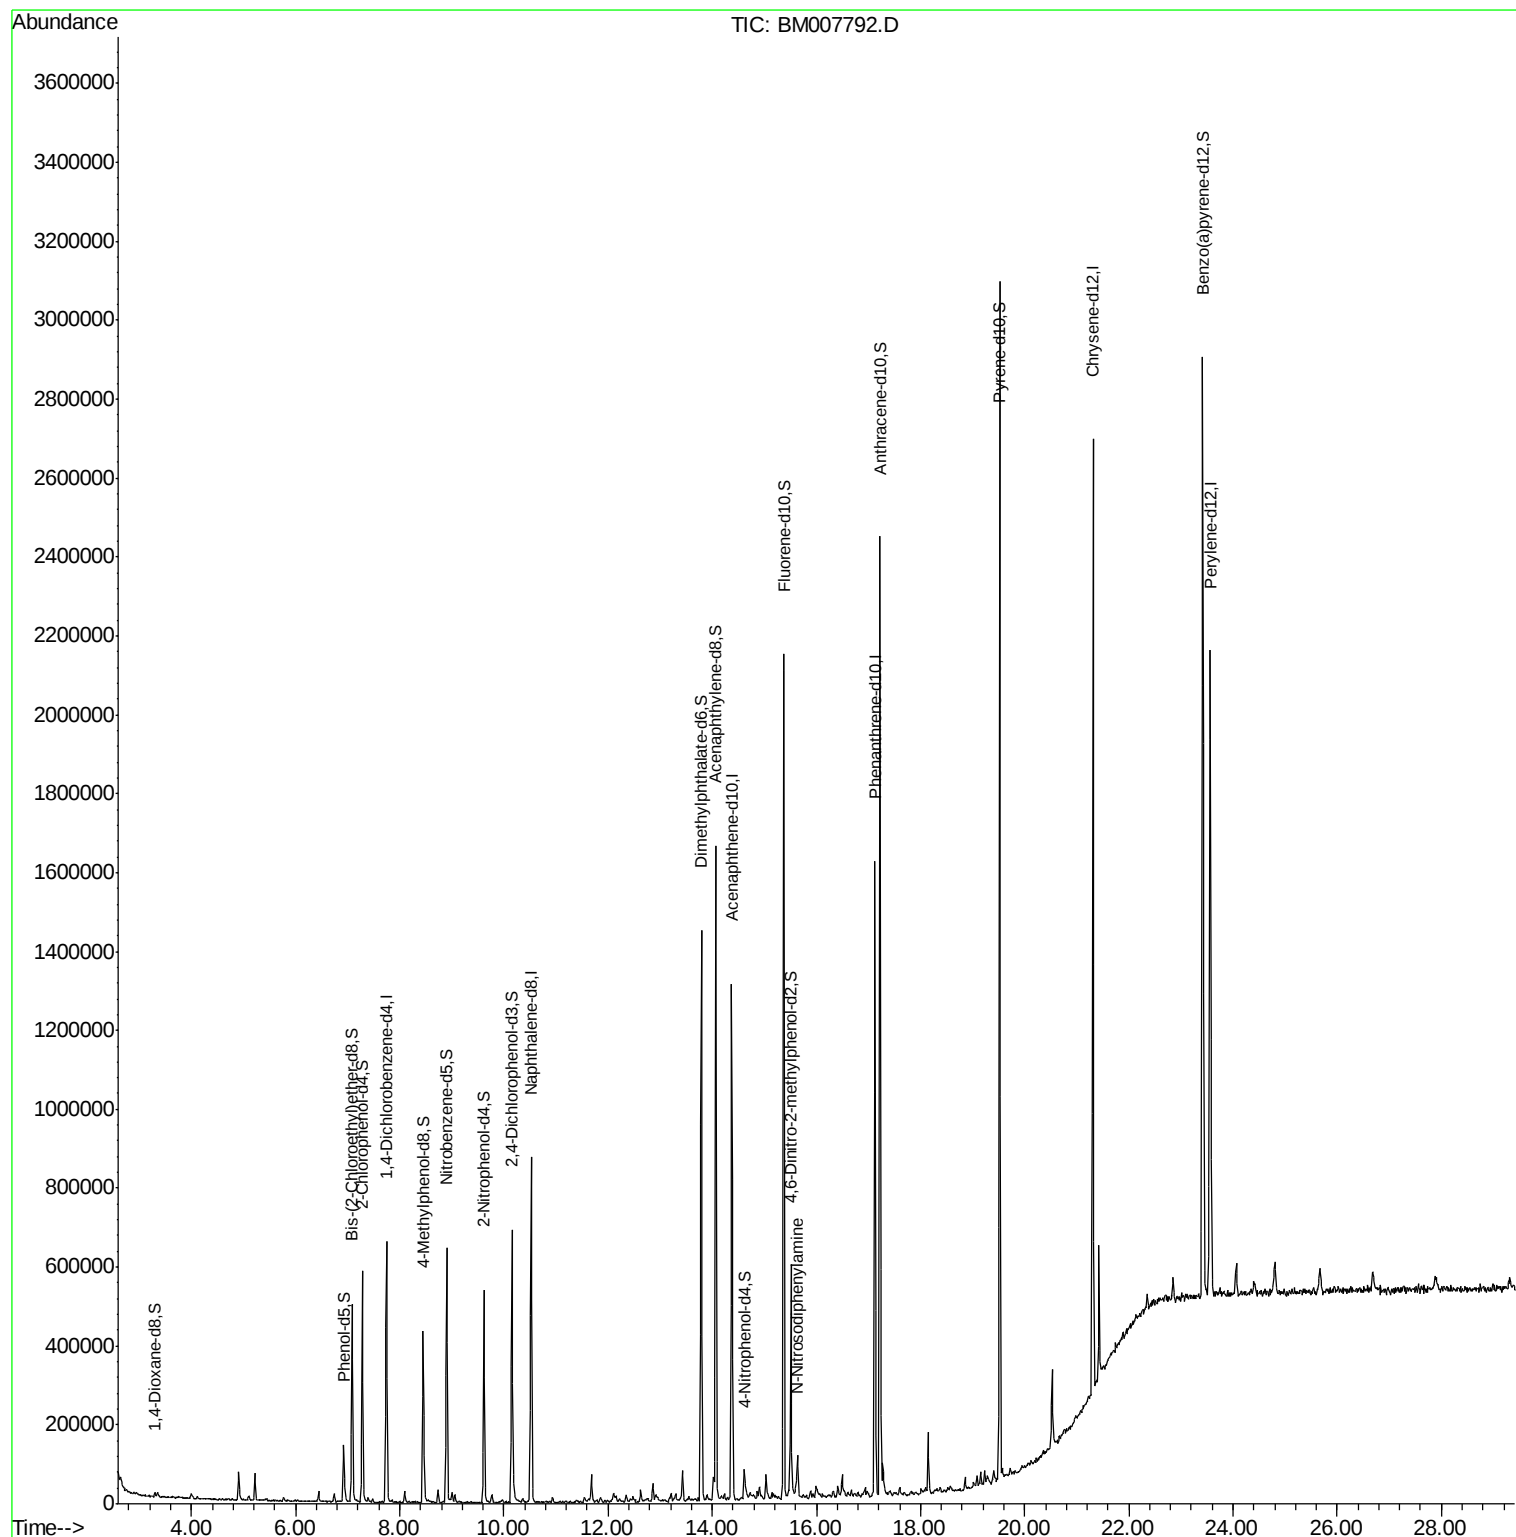


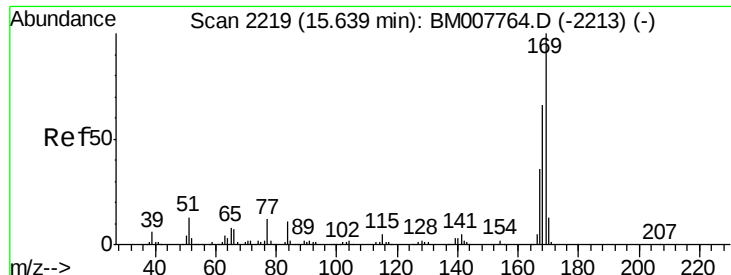

#64
 N-Nitrosodiphenylamine
 Concen: 1.06 ng/ul
 RT: 15.64 min Scan# 2219
 Delta R.T. -0.00 min
 Lab File: BM007792.D
 Acq: 09 Nov 2016 12:12

Instrument :
 BNA_M
 ClientSampleId :
 BBBM5

Tgt Ion:169 Resp: 27883
 Ion Ratio Lower Upper
 169 100
 168 65.7 52.6 79.0
 167 39.0 28.6 43.0

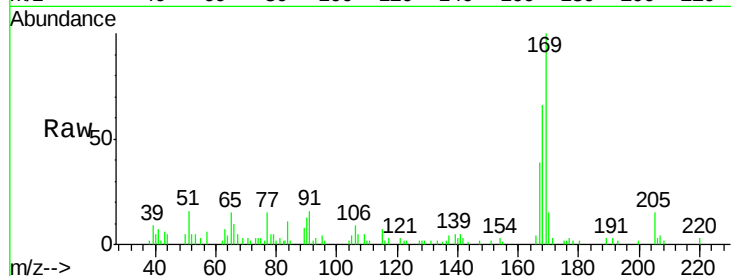

Abundance Ion 169.00 (168.70 to 169.70): E
 Ion 168.00 (167.70 to 168.70): E
 Ion 167.00 (166.70 to 167.70): E

