

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110916\
 Data File : BM007810.D
 Acq On : 09 Nov 2016 22:51
 Operator : UM/SJ
 Sample : H5594-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD4Q4

Quant Time: Nov 09 23:38:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:34:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	171899	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	637958	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	401586	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	786807	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	981496	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1020223	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	5262	1.31	ng/uL	0.00
5) Phenol-d5	6.92	99	87260	6.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	255972	32.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	277724	27.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	169134	16.29	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	169758	36.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	182605	37.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	312066	32.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	5150	0.47	ng/ul	0.03
43) Dimethylphthalate-d6	13.79	166	1015799	37.15	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	1233910	37.49	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	12814	2.96	ng/ul	0.02
57) Fluorene-d10	15.37	176	885034	36.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	139052	29.75	ng/ul	0.00
70) Anthracene-d10	17.22	188	1363358	38.45	ng/ul	0.00
76) Pyrene-d10	19.52	212	1559994	38.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1710819	38.41	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.79	165	5855	1.17	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110916\
Data File : BM007810.D
Acq On : 09 Nov 2016 22:51
Operator : UM/SJ
Sample : H5594-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD4Q4

Quant Time: Nov 09 23:38:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 23:34:58 2016
Response via : Initial Calibration

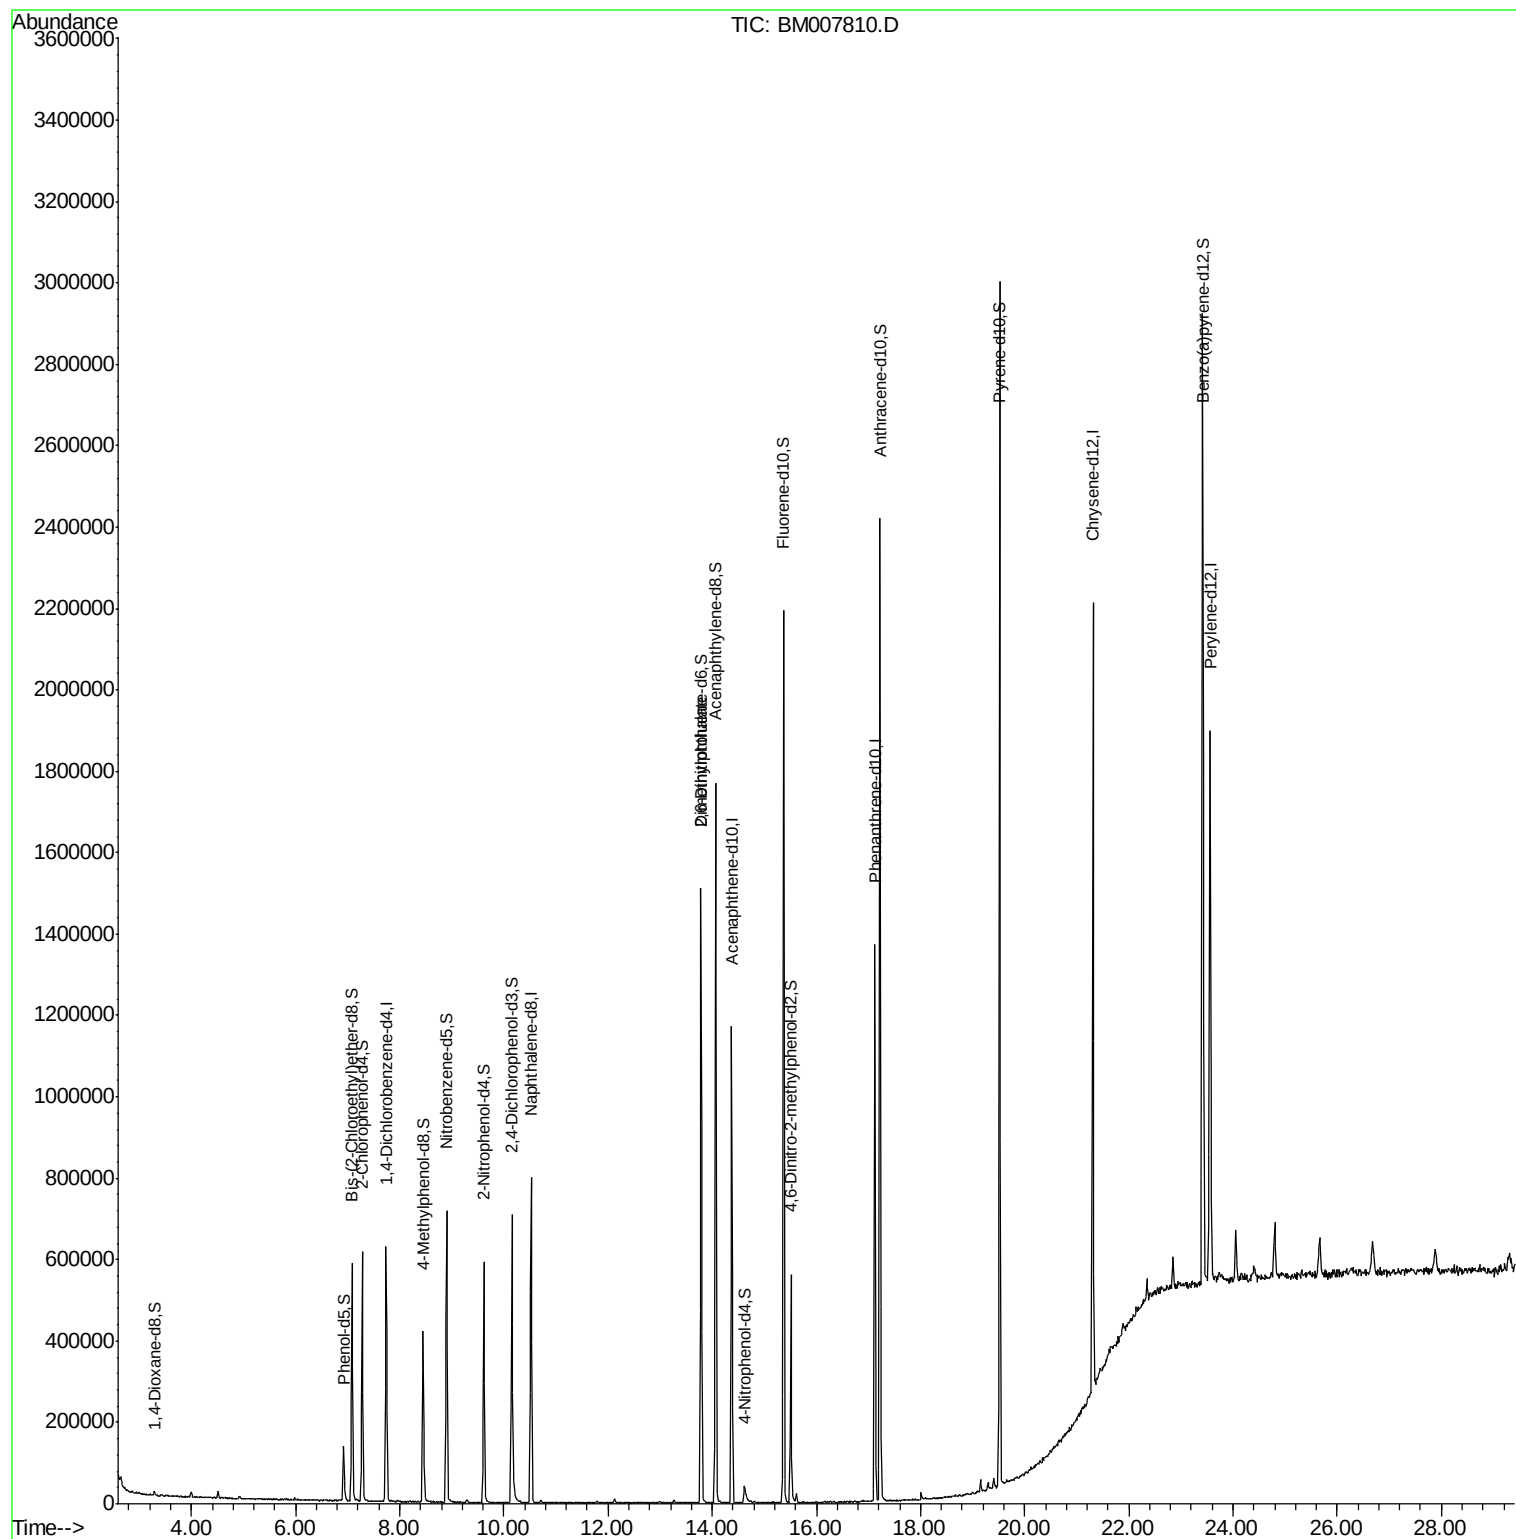

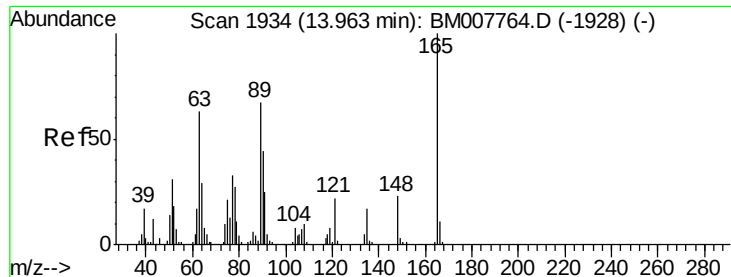

#45

2,6-Dinitrotoluene

Concen: 1.17 ng/ul

RT: 13.79 min Scan# 1905

Delta R.T. -0.17 min

Lab File: BM007810.D

Acq: 09 Nov 2016 22:51

Instrument :

BNA_M

ClientSampleId :

BD4Q4



Tgt Ion:165 Resp: 5855

Ion Ratio Lower Upper

165 100

89 0.0 46.6 69.8#

121 37.8 16.0 24.0#

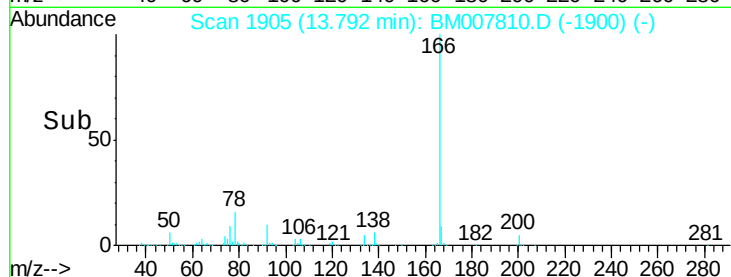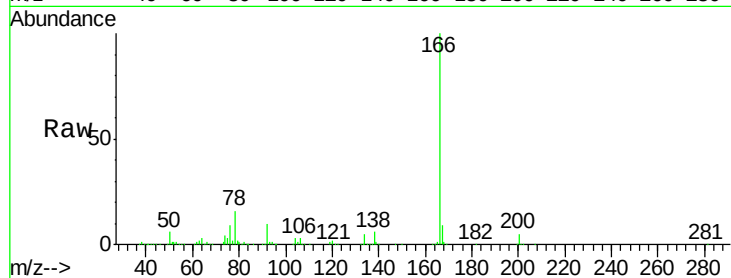

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

