

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110916\
 Data File : BM007812.D
 Acq On : 10 Nov 2016 00:02
 Operator : UM/SJ
 Sample : H5554-10DL 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N82DL

Quant Time: Nov 10 01:25:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:34:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	177185	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	697694	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	441150	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	863695	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	1089701	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1131909	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	2071	0.50	ng/uL	0.00
5) Phenol-d5	6.93	99	28980	2.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	19905	2.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	24379	2.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	21158	1.98	ng/ul	0.01
19) Nitrobenzene-d5	8.91	128	10919	2.17	ng/ul	0.01
22) 2-Nitrophenol-d4	9.62	143	10457	1.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	19469	1.86	ng/ul	0.03
29) 4-Chloroaniline-d4	10.69	131	15793	1.32	ng/ul	0.02
43) Dimethylphthalate-d6	13.80	166	72285	2.41	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	81019	2.24	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	1595	0.34	ng/ul	0.06
57) Fluorene-d10	15.37	176	64655	2.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	3175	0.62	ng/ul	0.02
70) Anthracene-d10	17.23	188	94526	2.43	ng/ul	0.00
76) Pyrene-d10	19.52	212	110602	2.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	123858	2.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
78) Butylbenzylphthalate	20.44	149	403004	20.12	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM110916\
Data File : BM007812.D
Acq On : 10 Nov 2016 00:02
Operator : UM/SJ
Sample : H5554-10DL 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N82DL

Quant Time: Nov 10 01:25:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 23:34:58 2016
Response via : Initial Calibration

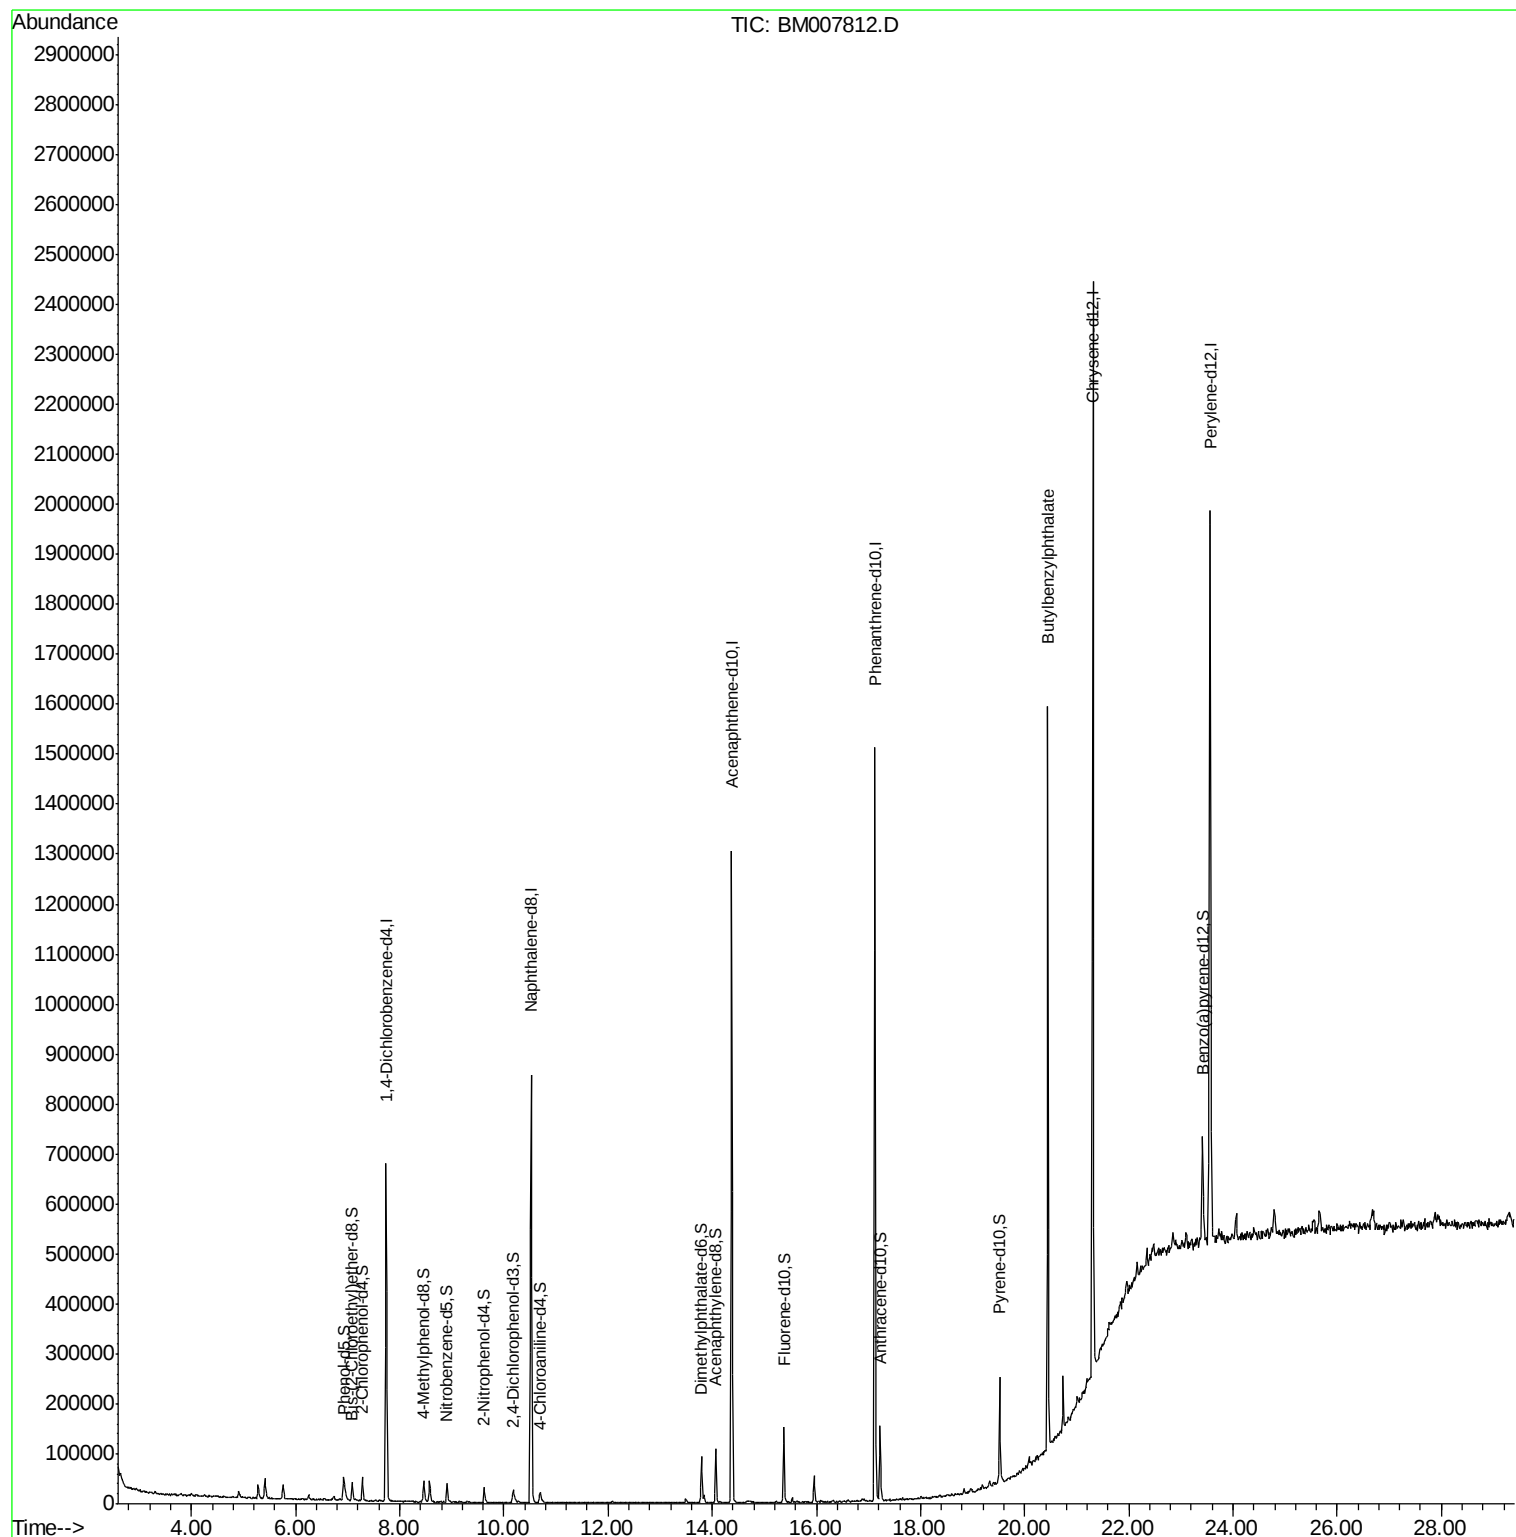

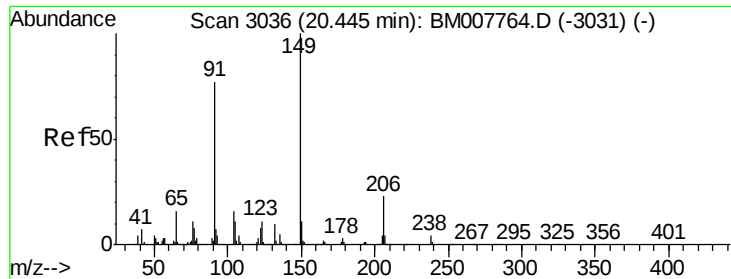

#78

Butylbenzylphthalate

Concen: 20.12 ng/ul

RT: 20.44 min Scan# 3036

Delta R.T. 0.00 min

Lab File: BM007812.D

Acq: 10 Nov 2016 00:02

Instrument :

BNA_M

ClientSampleId :

E5N82DL

Tgt Ion:149 Resp: 403004

Ion Ratio Lower Upper

149 100

91 76.0 57.3 85.9

206 23.7 18.6 27.8

