

Data Path : Z:\HPCHEM1\BNA M\DATA\BM110916\
 Data File : BM007801.D
 Acq On : 09 Nov 2016 17:32
 Operator : UM/SJ
 Sample : H5554-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N86

Manual Integrations
 APPROVED

umangi
 11/10/2016 8:42:33 AM

Quant Time: Nov 09 23:47:18 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM102016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:34:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	232801	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	880508	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	553620	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	1057794	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	1210411	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1230897	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	15695	2.89	ng/uL	0.00
5) Phenol-d5	6.92	99	275382	15.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	187082	17.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	231106	16.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	176107	12.53	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	118885	18.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	123256	18.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	205818	15.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	197934	13.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.79	166	708626	18.80	ng/ul	0.00
46) Acenaphthylene-d8	14.07	160	847044	18.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	45904m	7.70	ng/ul	0.01
57) Fluorene-d10	15.37	176	623529	18.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.51	200	58855	9.37	ng/ul	0.00
70) Anthracene-d10	17.22	188	889986	18.67	ng/ul	0.00
76) Pyrene-d10	19.52	212	1076860	21.65	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1082594	20.15	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	6.95	94	67953	3.68	ng/ul	99
44) Dimethylphthalate	13.84	163	80071	2.19	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM110916\
Data File : BM007801.D
Acq On : 09 Nov 2016 17:32
Operator : UM/SJ
Sample : H5554-14
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E5N86

Manual Integrations
APPROVED

umangi
11/10/2016 8:42:33 AM

Quant Time: Nov 09 23:47:18 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 23:34:58 2016
Response via : Initial Calibration

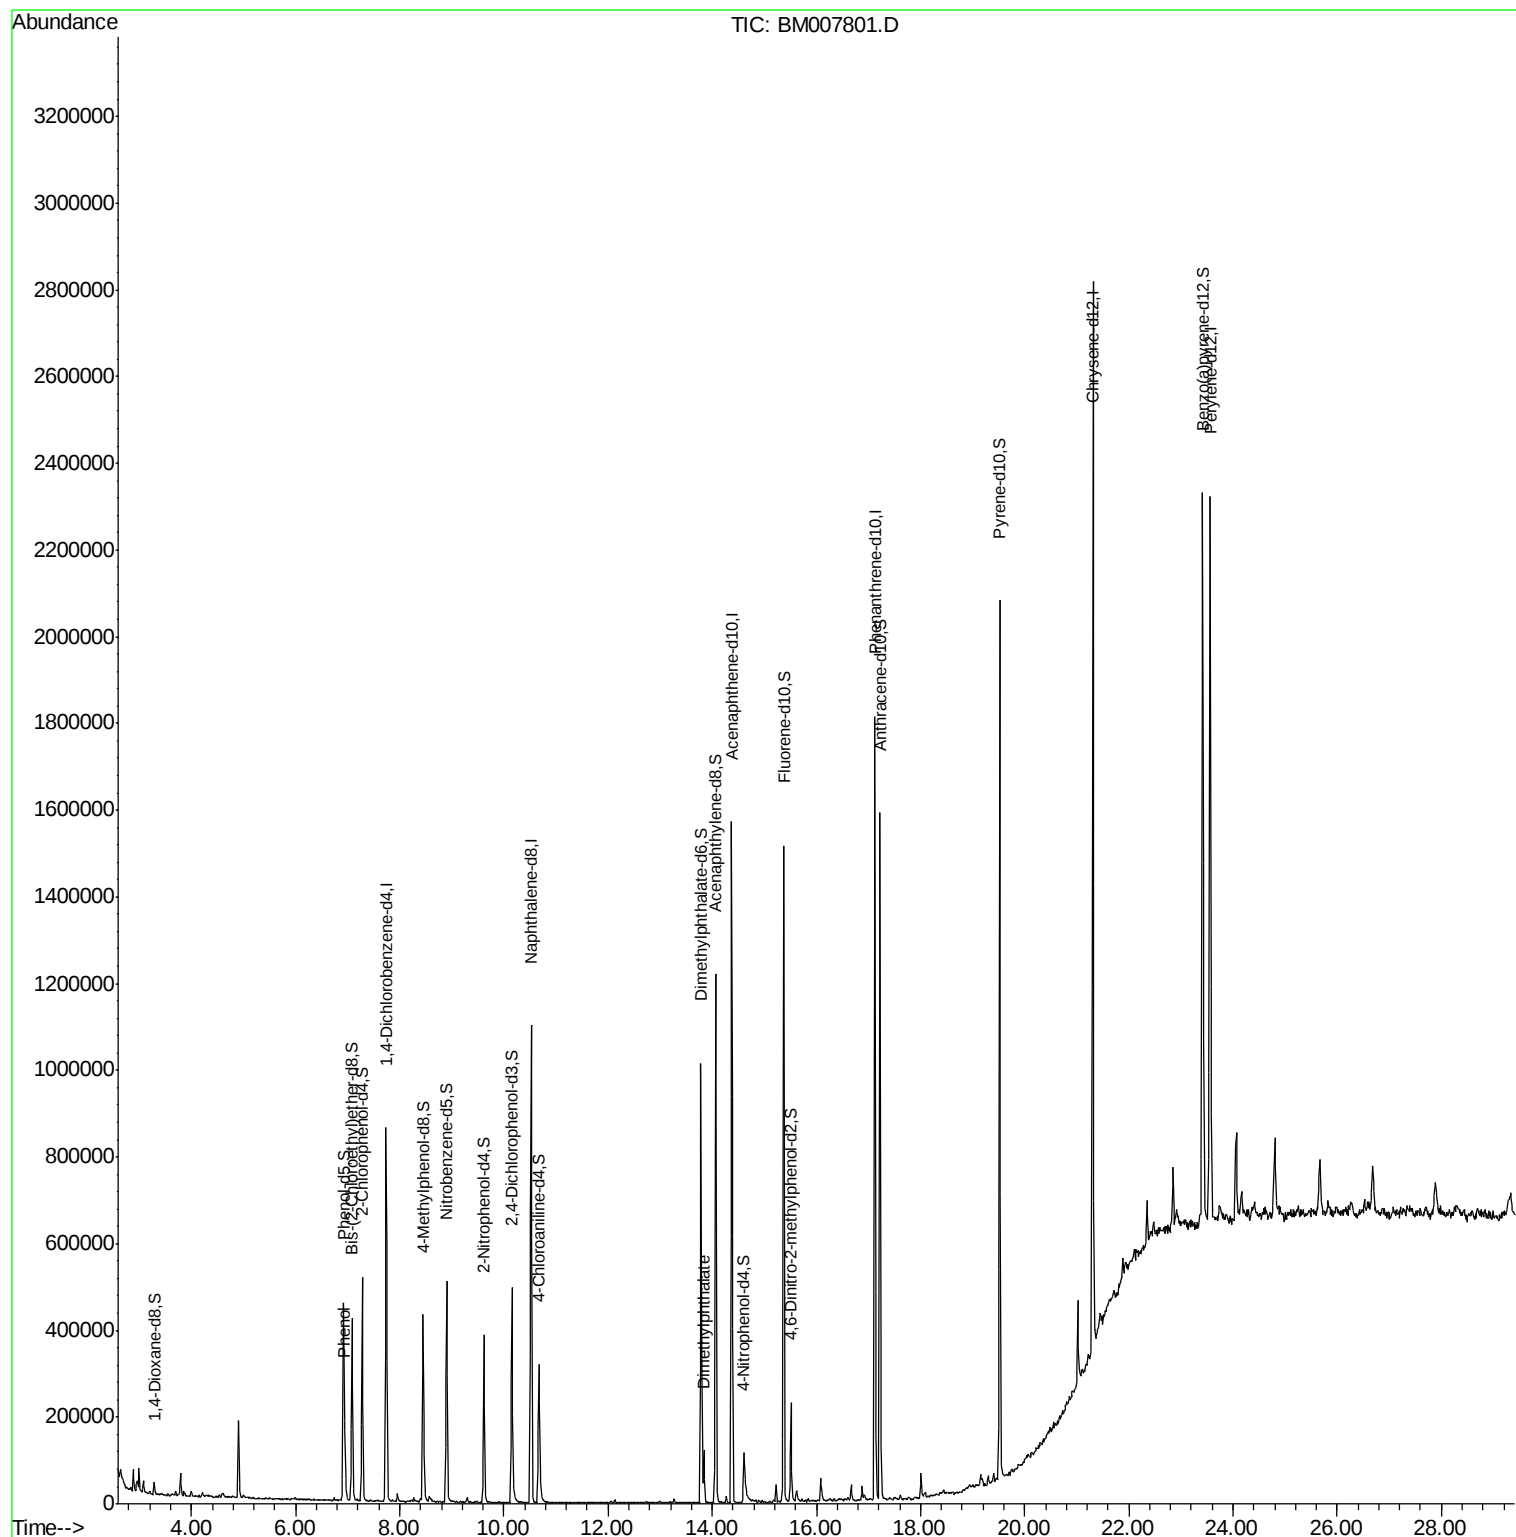

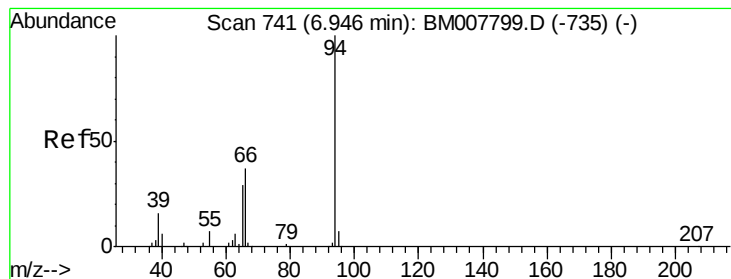

#6

Phenol

Concen: 3.68 ng/ul

RT: 6.95 min Scan# 741

Delta R.T. -0.00 min

Lab File: BM007801.D

Acq: 09 Nov 2016 17:32

Instrument :

BNA_M





ClientSampled :

E5N86

Tot Ion:	94	Resp:	67953
Ion	Ratio	Lower	Upper
94	100		
65	29.0	23.9	35.9
66	41.4	33.5	50.3

Manual Integrations
APPROVED

umangi
11/10/2016 8:42:33 AM

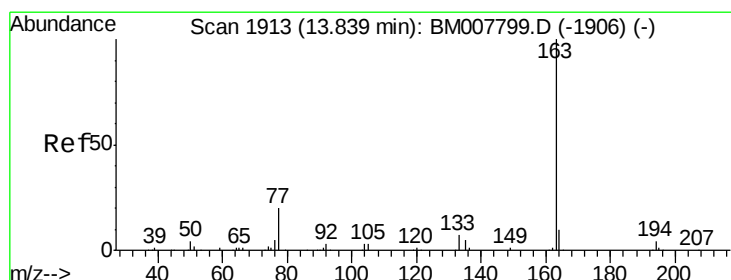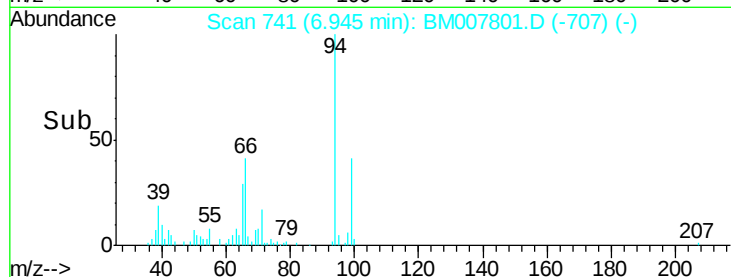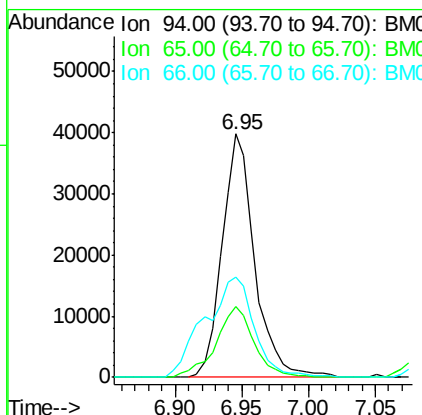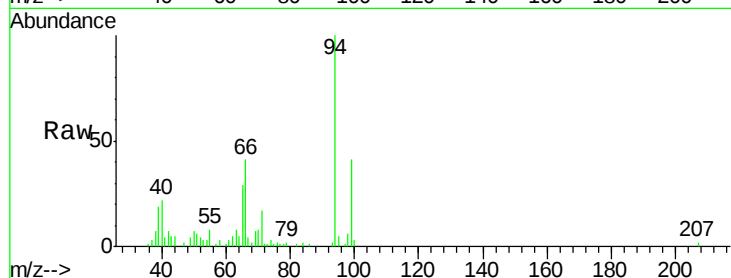

#44

Dimethylphthalate

Concen: 2.19 ng/ul

RT: 13.84 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BM007801.D

Acq: 09 Nov 2016 17:32

Tgt Ion:	163	Resp:	80071
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.2
164	9.9	7.8	11.8

