




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
 Data File : BM027757.D
 Acq On : 09 Nov 2020 14:55
 Operator : JU/CG
 Sample : L4661-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R05

Manual Integrations
 APPROVED

mohammad
 11/10/2020 12:01:21 PM

Quant Time: Nov 10 06:34:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 06:30:49 2020
 Response via : Initial Calibration

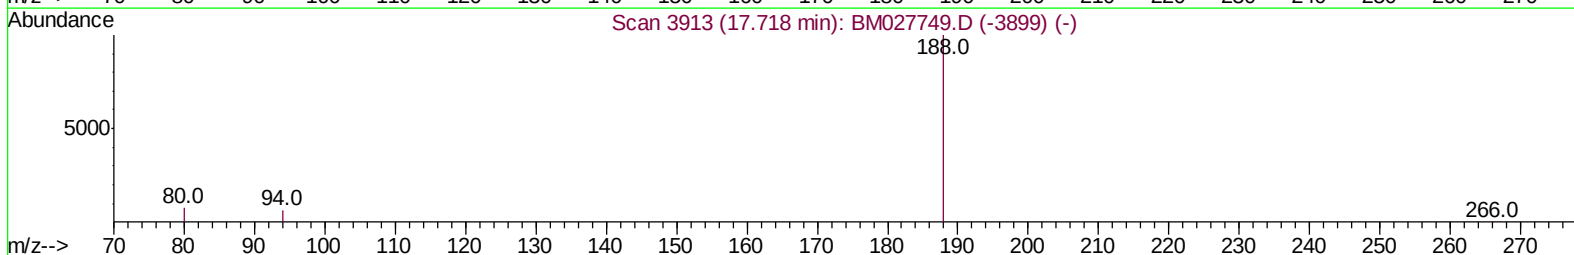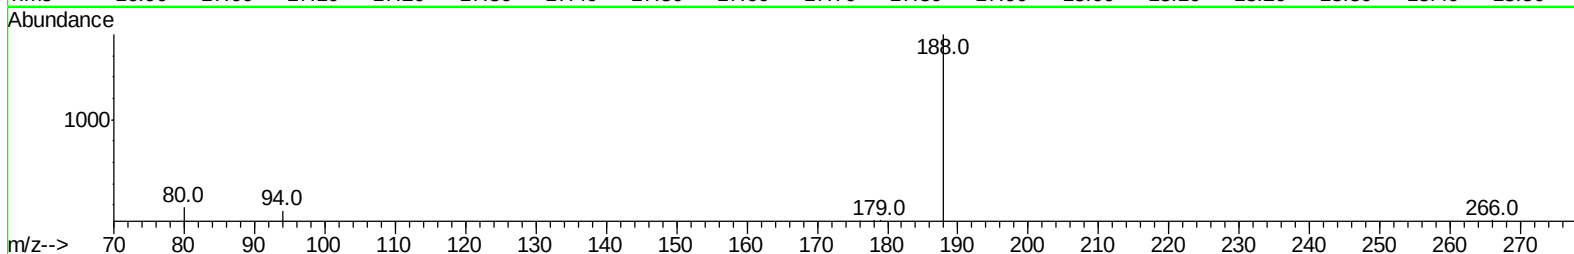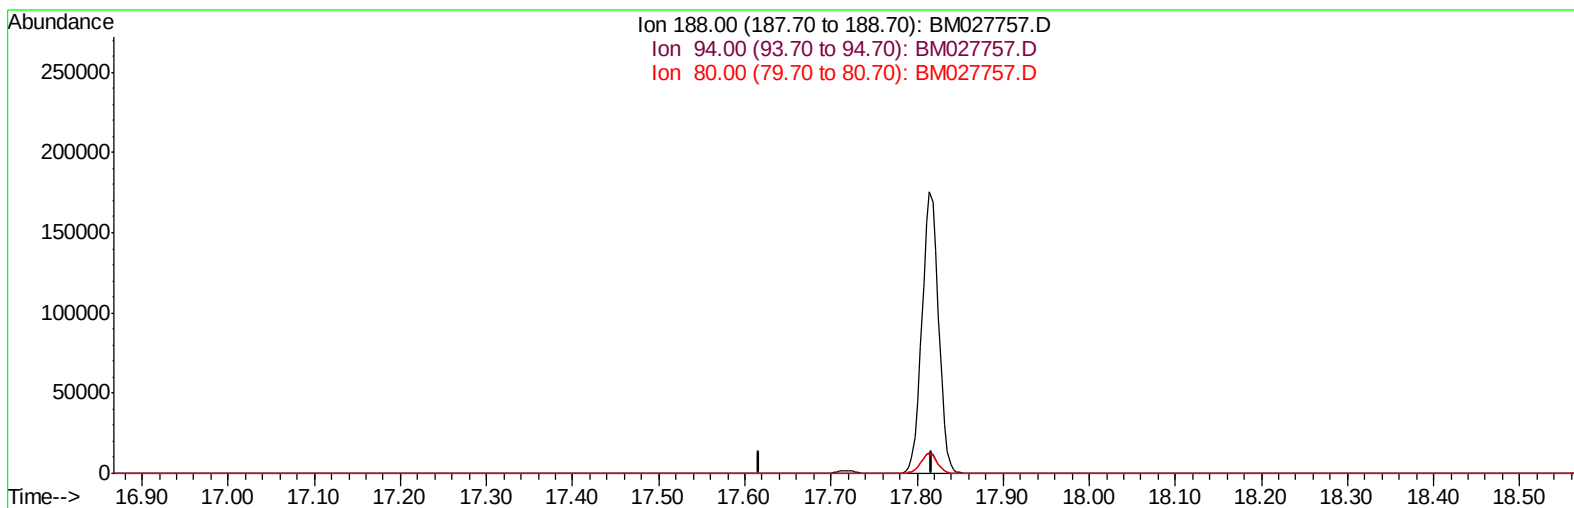

TIC: BM027757.D

(10) Phenanthrene-d10 (I)

17.718min (-17.718) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.00	0.00#
80.00	10.40	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
 Data File : BM027757.D
 Acq On : 09 Nov 2020 14:55
 Operator : JU/CG
 Sample : L4661-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R05

Manual Integrations
 APPROVED

mohammad
 11/10/2020 12:01:21 PM

Quant Time: Nov 10 06:34:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 06:30:49 2020
 Response via : Initial Calibration

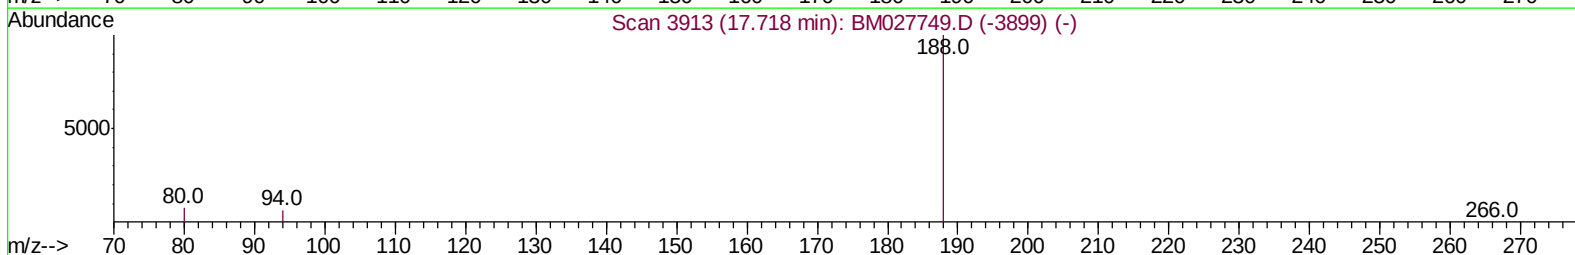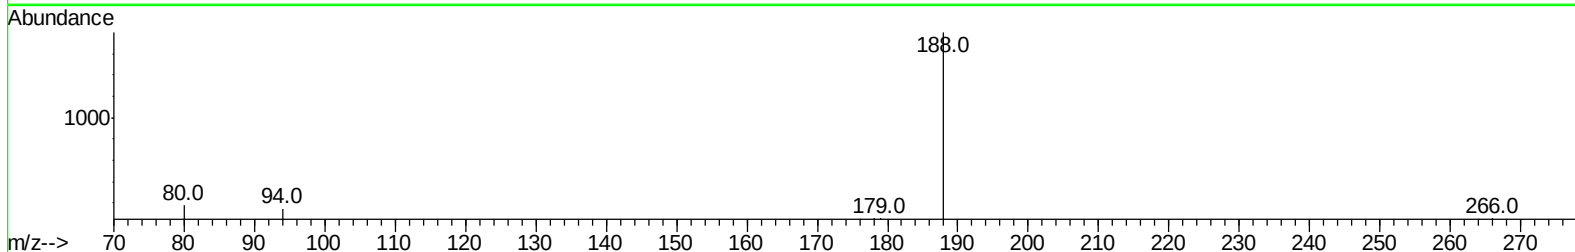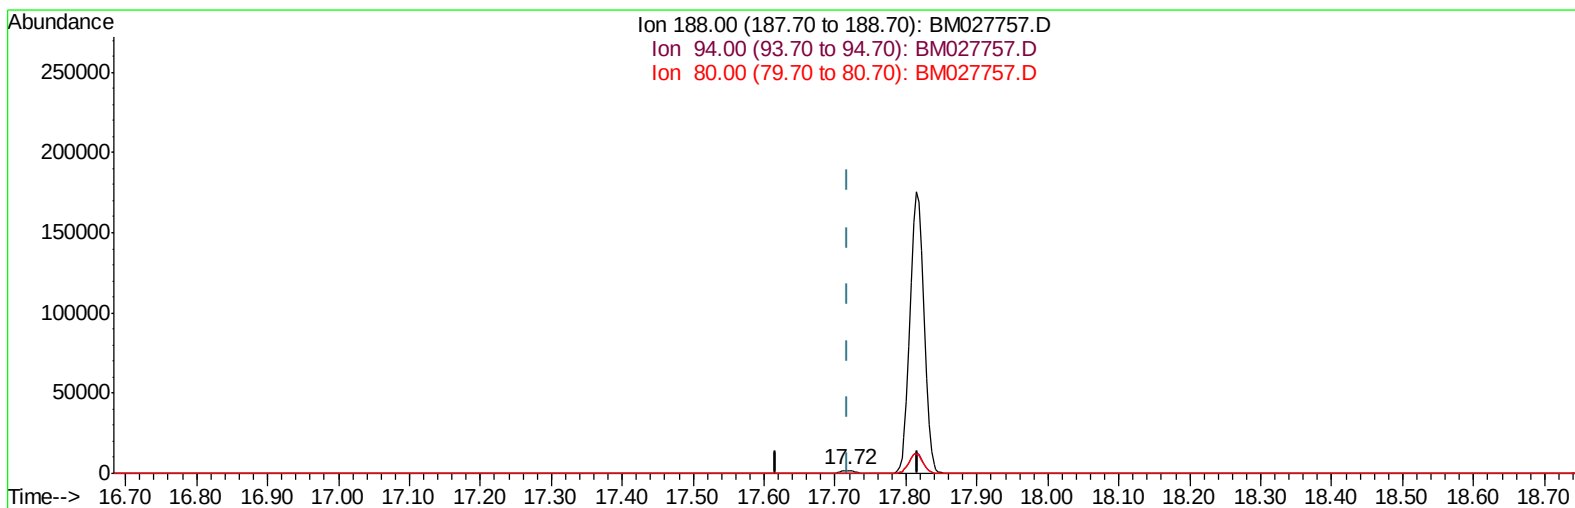

TIC: BM027757.D

(10) Phenanthrene-d10 (I)

17.718min (-0.000) 0.40ng/ul m

response 2437

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	8.29
80.00	10.40	9.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
 Data File : BM027757.D
 Acq On : 09 Nov 2020 14:55
 Operator : JU/CG
 Sample : L4661-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R05

Manual Integrations
 APPROVED

mohammad
 11/10/2020 12:01:21 PM

Quant Time: Nov 10 06:55:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 06:30:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	388	0.40	ng/ul	0.00
2) Naphthalene-d8	11.23	136	1359	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.00	164	1117	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.72	188	2437m	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	2860	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	2929	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.79	152	803	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	3284	0.45	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
Data File : BM027757.D
Acq On : 09 Nov 2020 14:55
Operator : JU/CG
Sample : L4661-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4R05

Quant Time: Nov 10 06:55:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 06:30:49 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
11/10/2020 12:01:21 PM

