




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
 Data File : BM027759.D
 Acq On : 09 Nov 2020 16:08
 Operator : JU/CG
 Sample : L4661-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R02

Manual Integrations
 APPROVED

mohammad
 11/10/2020 12:01:26 PM

Quant Time: Nov 10 06:34:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 06:30:49 2020
 Response via : Initial Calibration

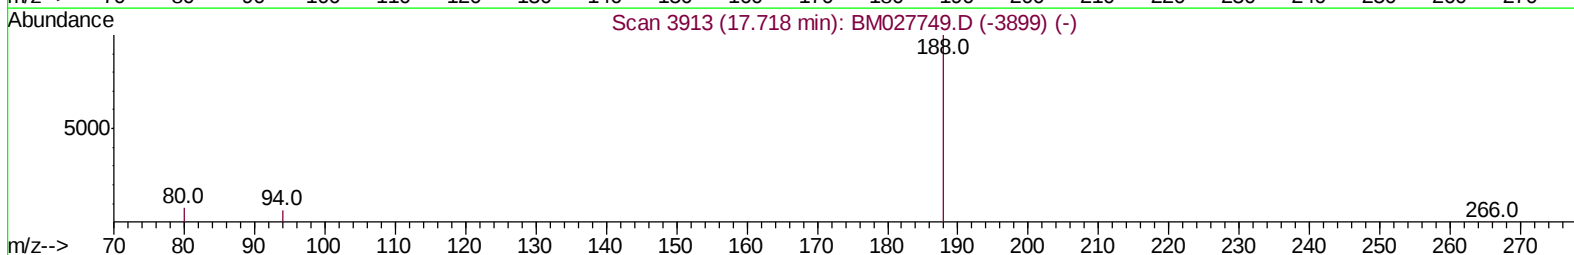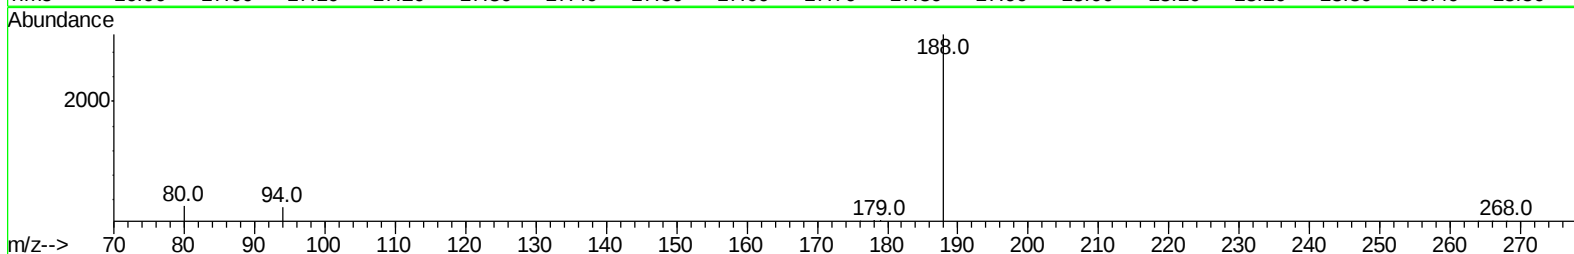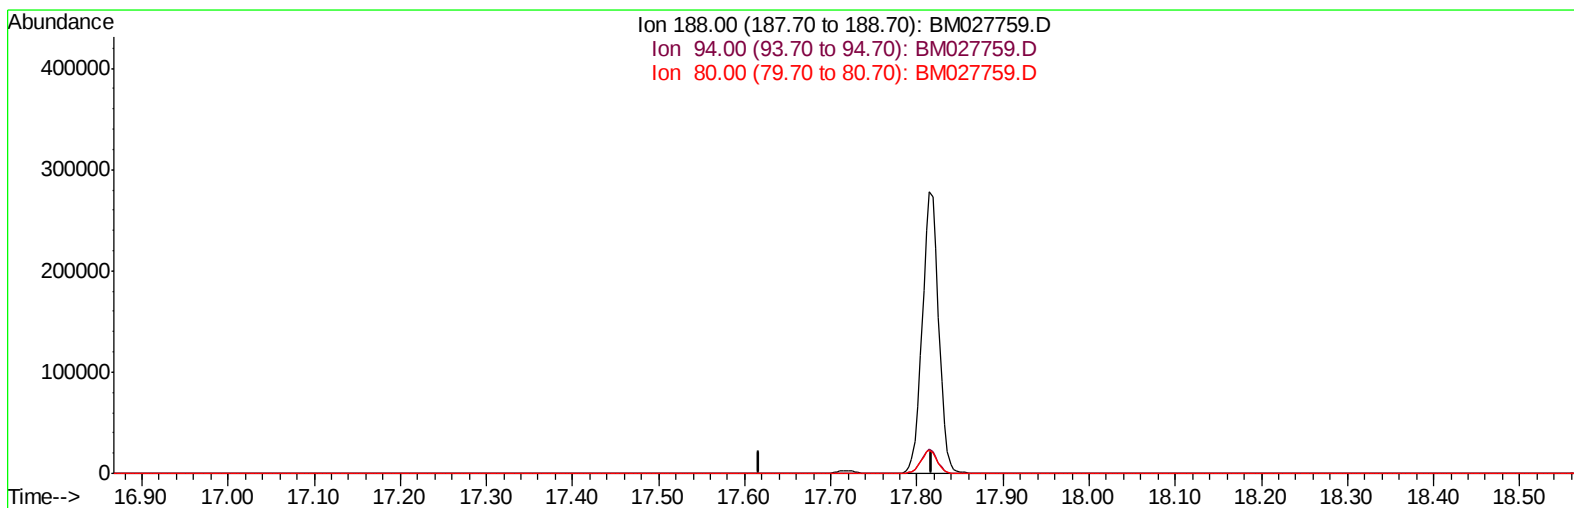

TIC: BM027759.D

(10) Phenanthrene-d10 (I)

17.718min (-17.718) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.00	0.00#
80.00	10.40	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
 Data File : BM027759.D
 Acq On : 09 Nov 2020 16:08
 Operator : JU/CG
 Sample : L4661-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R02

Manual Integrations
 APPROVED

mohammad
 11/10/2020 12:01:26 PM

Quant Time: Nov 10 06:34:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 06:30:49 2020
 Response via : Initial Calibration

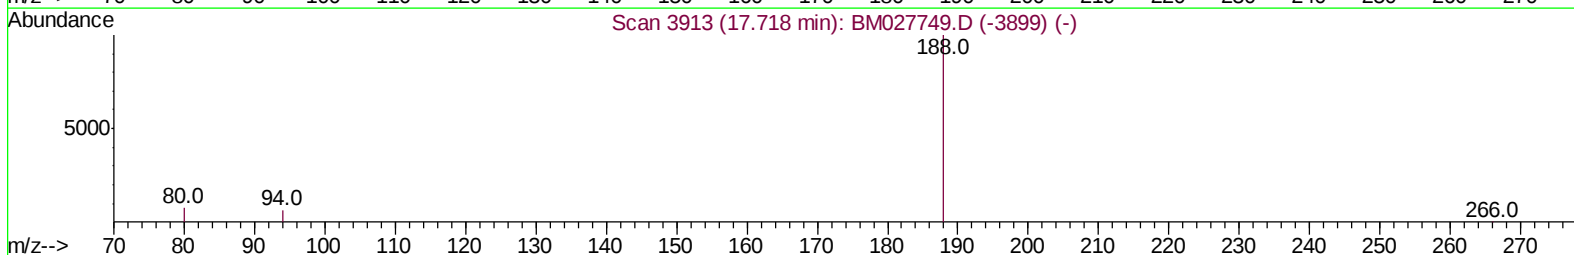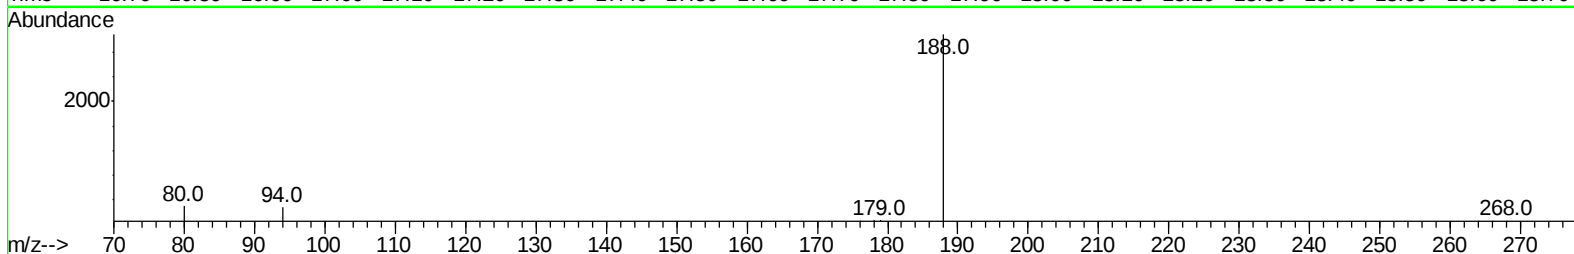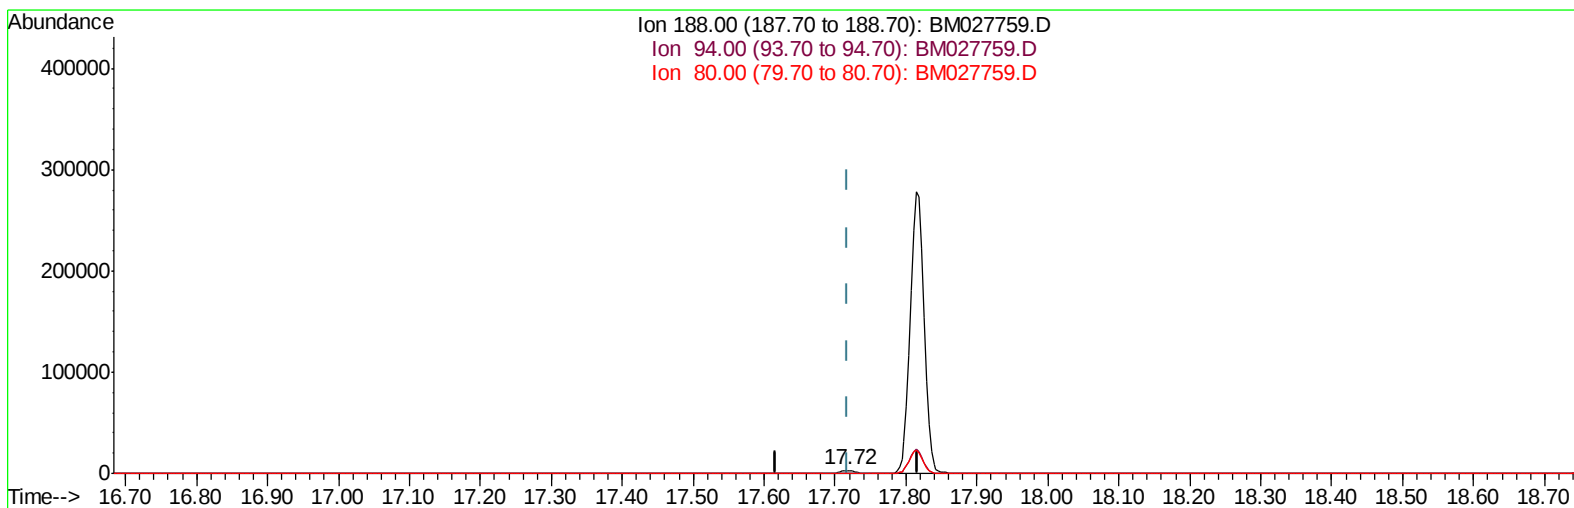

TIC: BM027759.D

(10) Phenanthrene-d10 (I)

17.718min (-0.000) 0.40ng/ul m

response 4207

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	8.77
80.00	10.40	9.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
 Data File : BM027759.D
 Acq On : 09 Nov 2020 16:08
 Operator : JU/CG
 Sample : L4661-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R02

Manual Integrations
 APPROVED

mohammad
 11/10/2020 12:01:26 PM

Quant Time: Nov 10 07:01:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 06:30:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	888	0.40	ng/ul	0.00
2) Naphthalene-d8	11.23	136	3319	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.00	164	2130	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.72	188	4207m	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	3723	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	3389	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.79	152	1620	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	4366	0.35	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110920\
Data File : BM027759.D
Acq On : 09 Nov 2020 16:08
Operator : JU/CG
Sample : L4661-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4R02

Quant Time: Nov 10 07:01:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM02.4-EPA-SIM-BM110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 06:30:49 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
11/10/2020 12:01:26 PM

