


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110921\  
Data File : BM032990.D  
Acq On : 11 Nov 2021 14:19  
Operator : CG/JU  
Sample : M4615-01  
Misc :  
ALS Vial : 86 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
C0V00

## Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021  
Supervised By :mohammad ahmed 11/17/2021

Quant Time: Nov 11 15:34:38 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM110921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 11 13:40:18 2021  
Response via : Initial Calibration

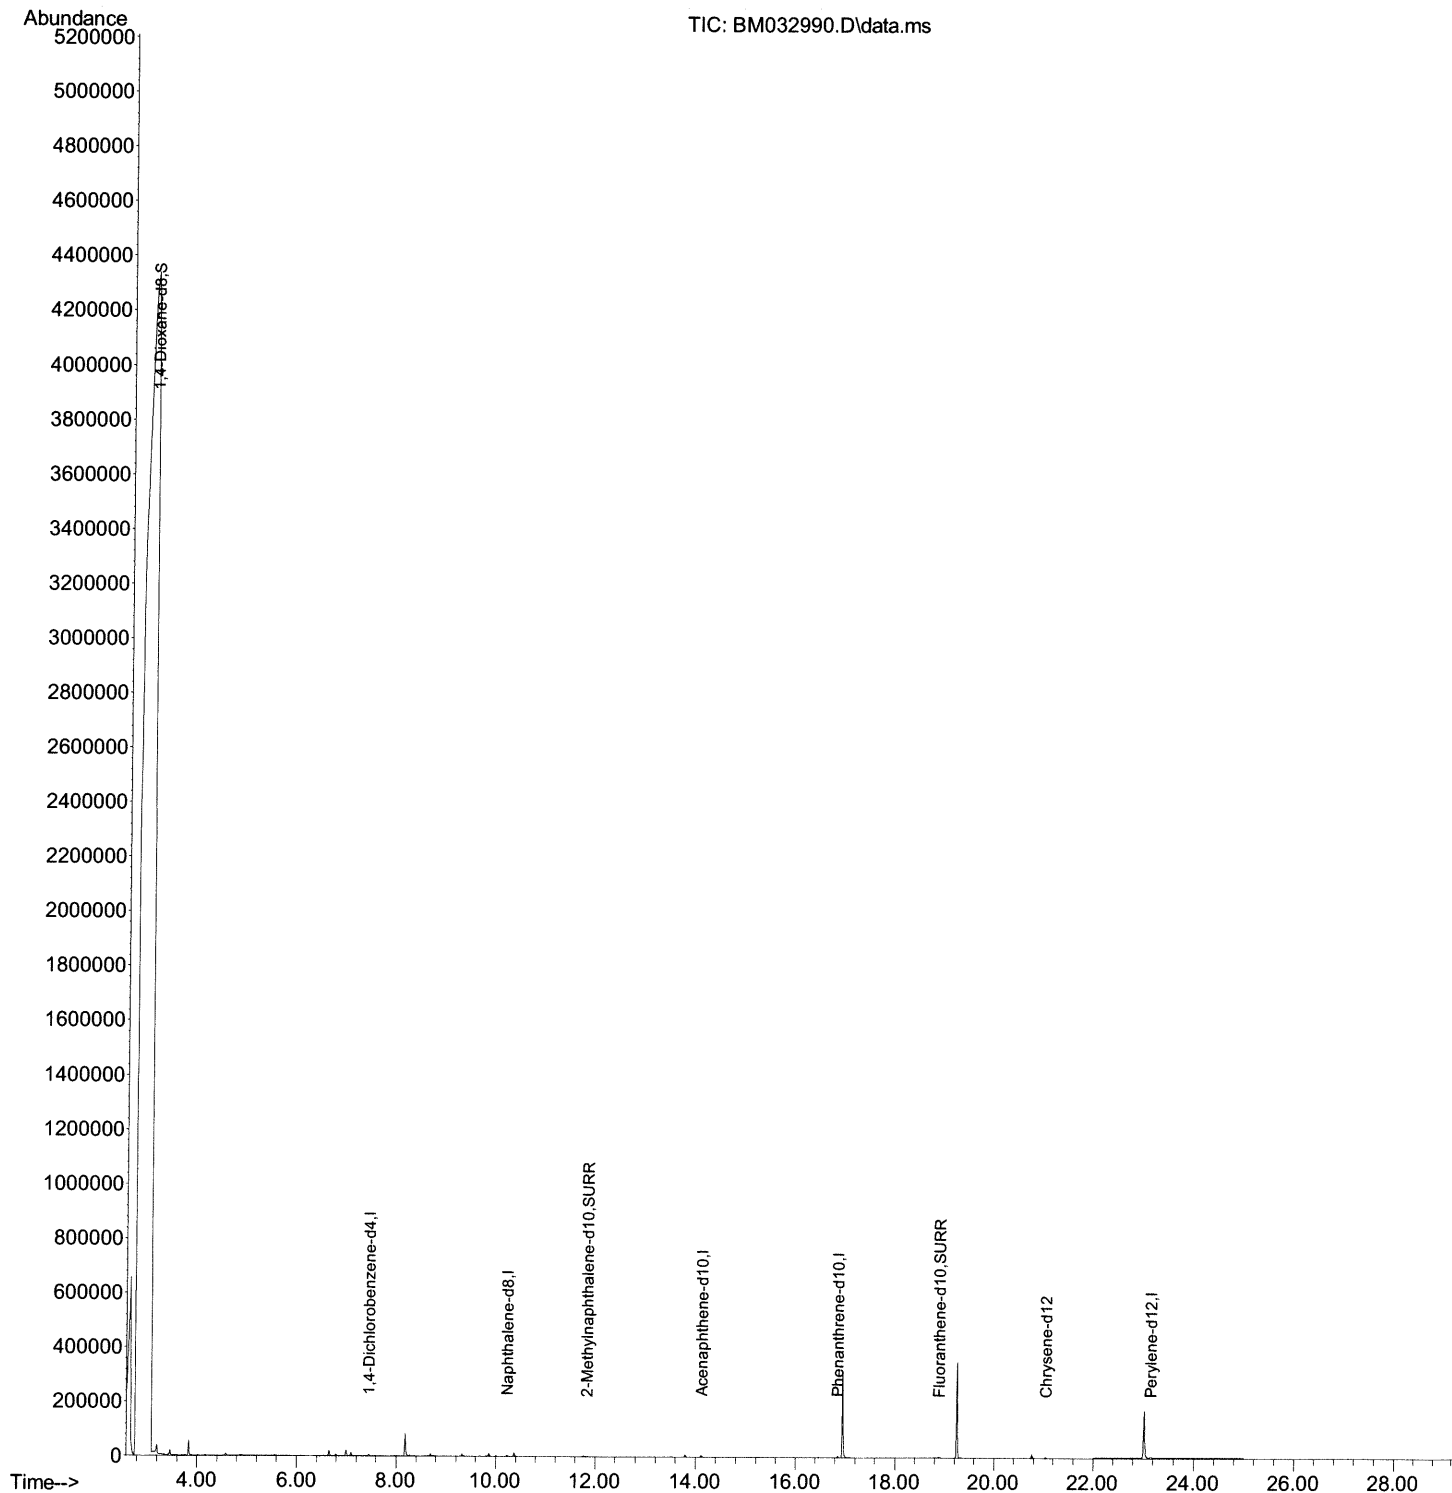

# Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110921\  
 Data File : BM032990.D  
 Acq On : 11 Nov 2021 14:19  
 Operator : CG/JU  
 Sample : M4615-01  
 Misc :  
 ALS Vial : 86 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0V00

Manual IntegrationsAPPROVED

Quant Time: Nov 11 15:34:38 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM110921.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 11 13:40:18 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/11/2021  
 Supervised By :mohammad ahmed 11/17/2021

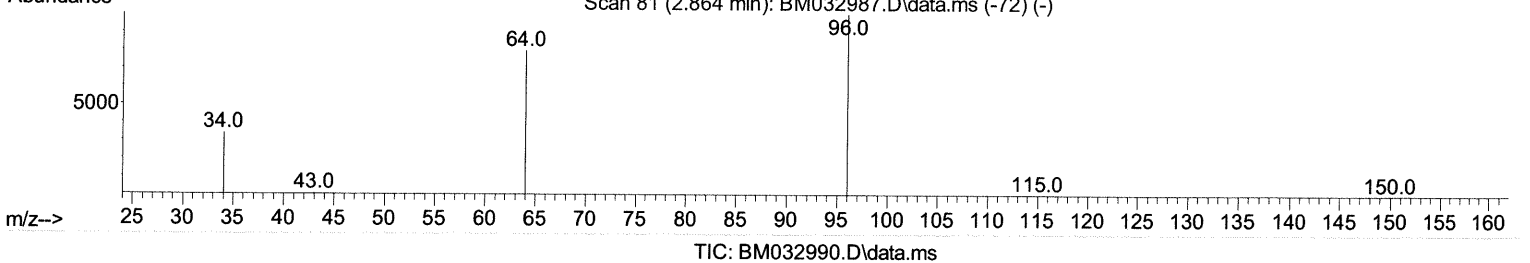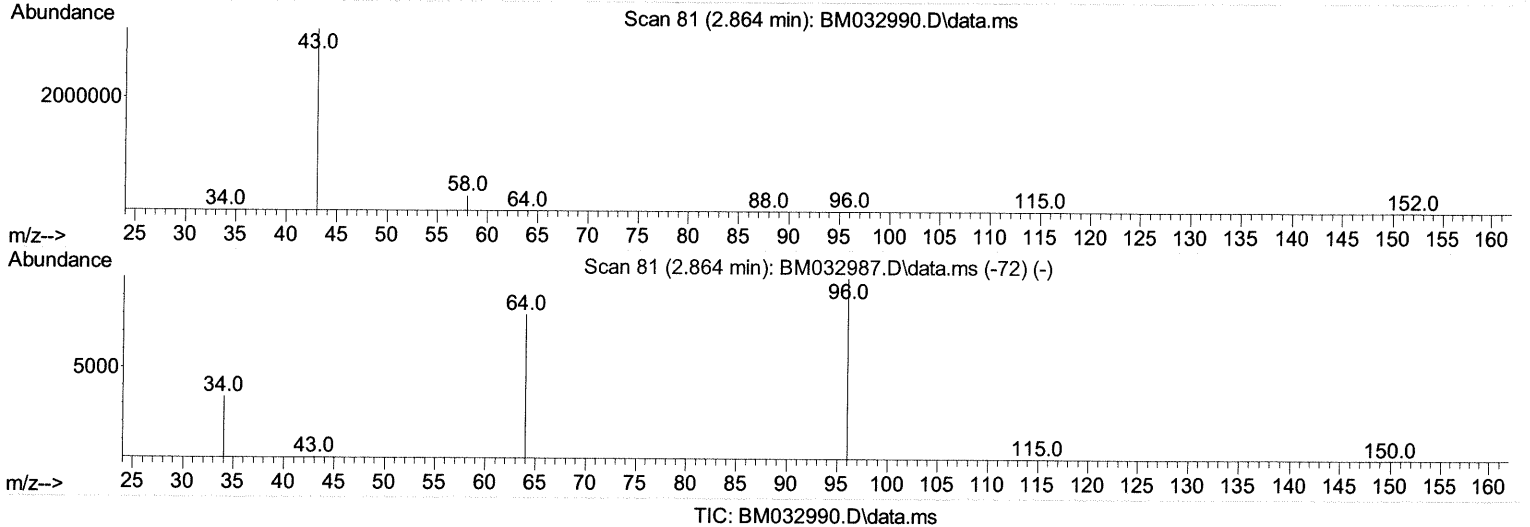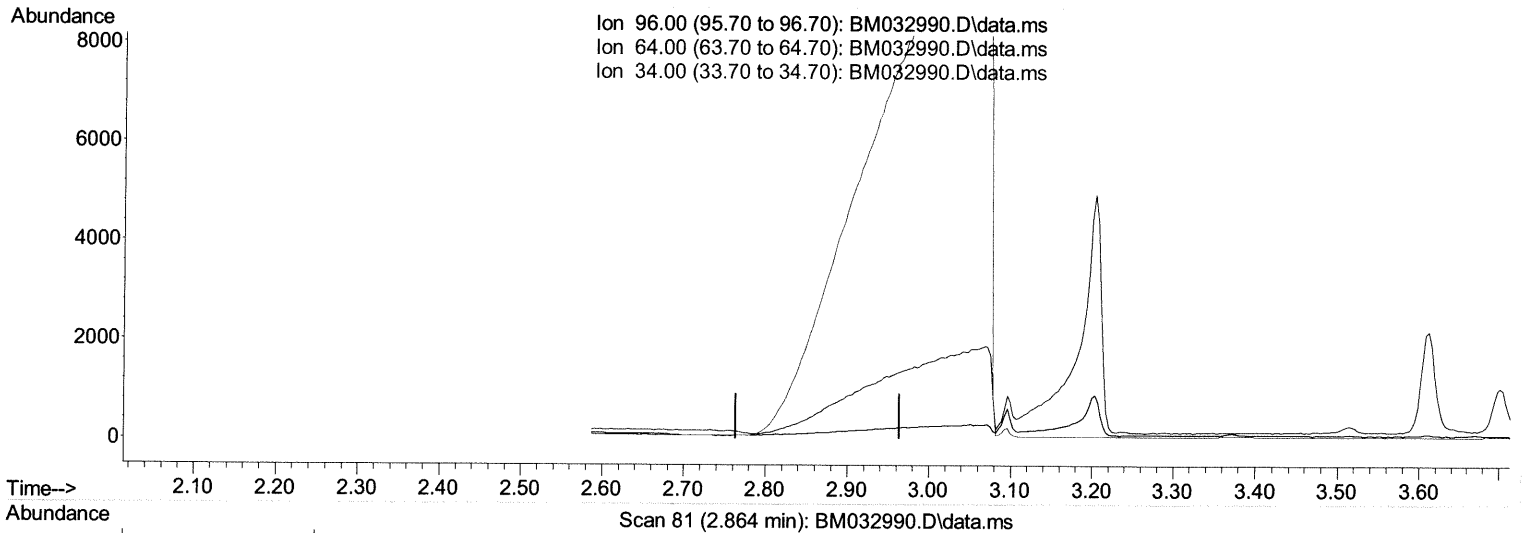

TIC: BM032990.D\data.ms

(3) 1,4-Dioxane-d8 (S)

2.864min (-2.864) 0.00 ng/ul

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	69.00	0.00#
34.00	32.60	0.00#
0.00	0.00	0.00

# Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110921\  
 Data File : BM032990.D  
 Acq On : 11 Nov 2021 14:19  
 Operator : CG/JU  
 Sample : M4615-01  
 Misc :  
 ALS Vial : 86 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0V00

Manual IntegrationsAPPROVED

Quant Time: Nov 11 15:34:38 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM110921.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 11 13:40:18 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/11/2021  
 Supervised By :mohammad ahmed 11/17/2021

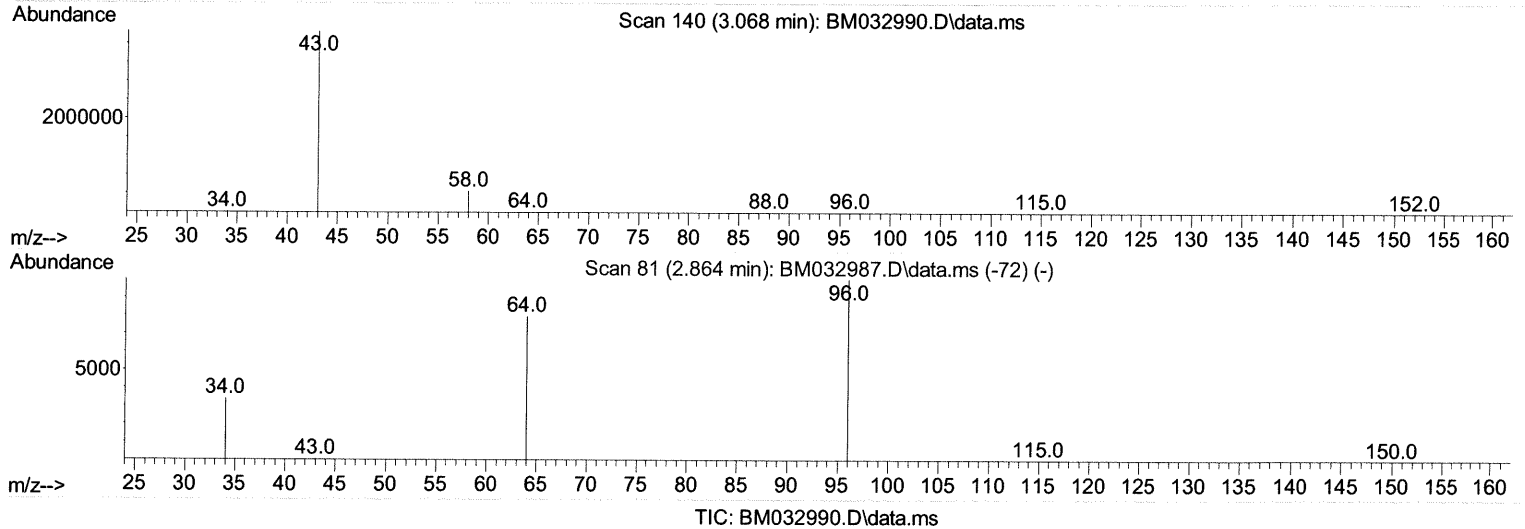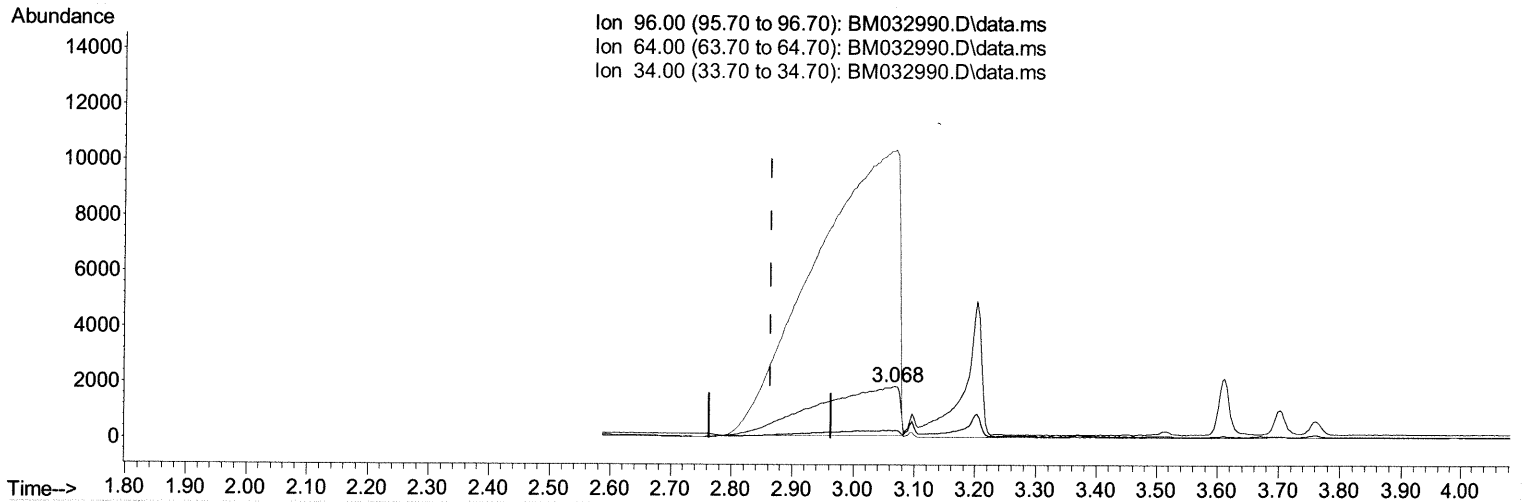

(3) 1,4-Dioxane-d8 (S)

3.068min (+ 0.204) 6.01 ng/ul m 11/13/21 JU

response 16473

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	69.00	15.76#
34.00	32.60	553.41#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110921\  
 Data File : BM032990.D  
 Acq On : 11 Nov 2021 14:19  
 Operator : CG/JU  
 Sample : M4615-01  
 Misc :  
 ALS Vial : 86 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 C0V00

## Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/11/2021  
 Supervised By :mohammad ahmed 11/17/2021

Quant Time: Nov 11 15:34:38 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM110921.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Nov 11 13:40:18 2021  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	2147	0.400	ng/ul	0.00
4) Naphthalene-d8	10.230	136	6989	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.114	164	3844	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.858	188	7284	0.400	ng/ul	0.00
17) Chrysene-d12	21.050	240	4401	0.400	ng/ul	0.00
23) Perylene-d12	23.154	264	3929	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.068	96	16473m	6.008	ng/ul	0.20
6) 2-Methylnaphthalene-d10	11.831	152	2186	0.220	ng/ul	0.00
18) Fluoranthene-d10	18.889	212	3718	0.279	ng/ul	0.00

Target Compounds Qvalue

-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed