

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032915.D
 Acq On : 09 Nov 2021 15:05
 Operator : CG/JU
 Sample : M4532-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB862

Quant Time: Nov 09 15:36:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.466	152	1491	0.400	ng/ul	0.00
4) Naphthalene-d8	10.240	136	5472	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.126	164	3414	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.866	188	7217	0.400	ng/ul	0.00
17) Chrysene-d12	21.060	240	5856	0.400	ng/ul	0.00
23) Perylene-d12	23.169	264	4836	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.865	96	1389	0.730	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.841	152	2887	0.372	ng/ul	0.00
18) Fluoranthene-d10	18.897	212	7230	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	2.896	88	8643	4.420	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032915.D
Acq On : 09 Nov 2021 15:05
Operator : CG/JU
Sample : M4532-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB862


Quant Time: Nov 09 15:36:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

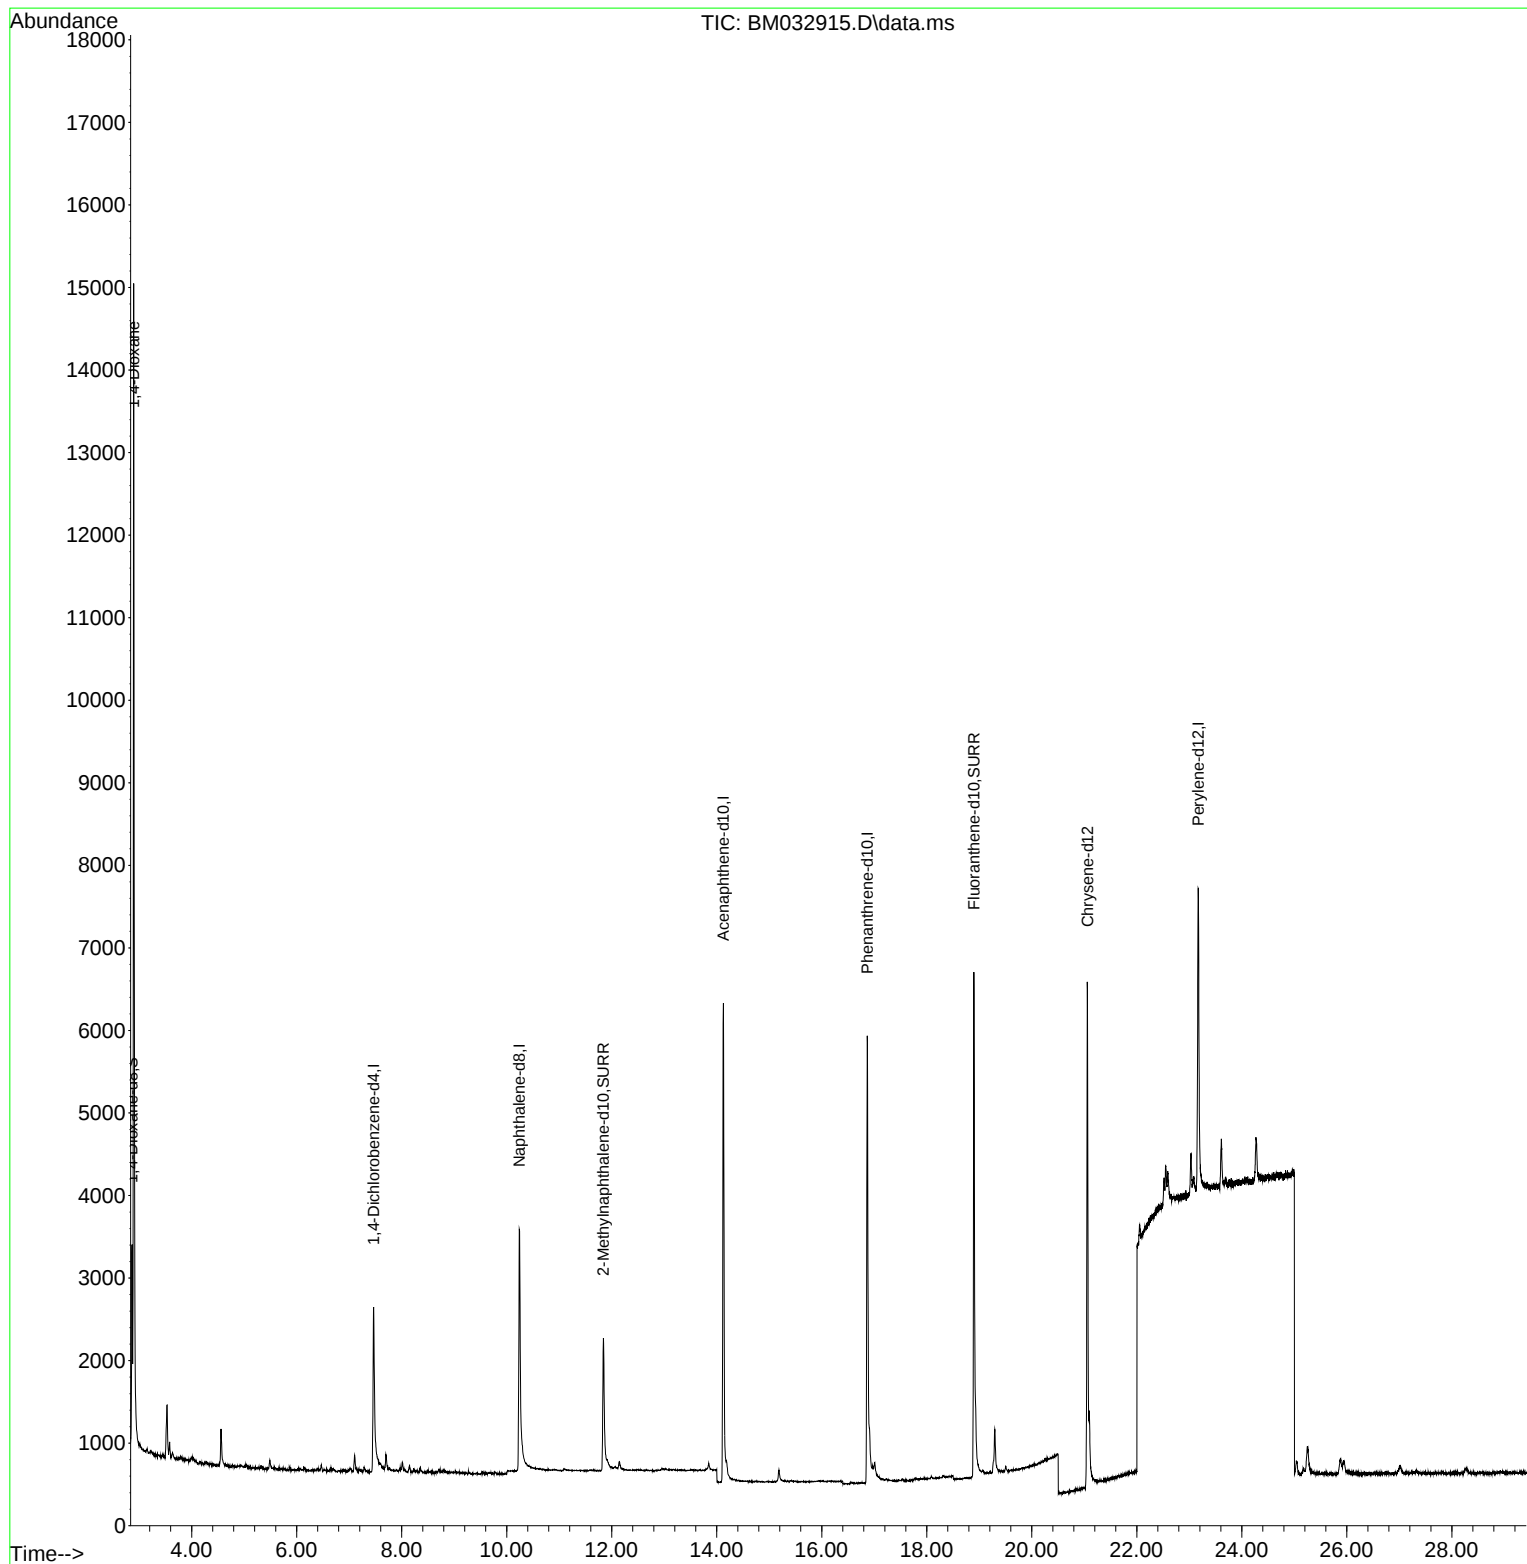


Abundance Scan 20 (2.903 min): BM032909.D\data.ms (-12)

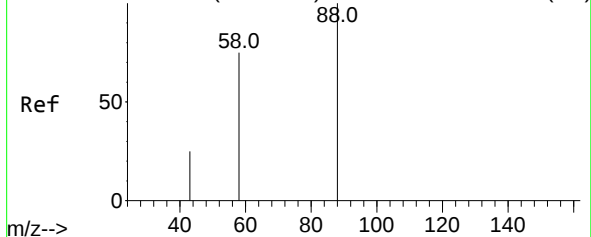

Abundance Scan 18 (2.896 min): BM032915.D\data.ms

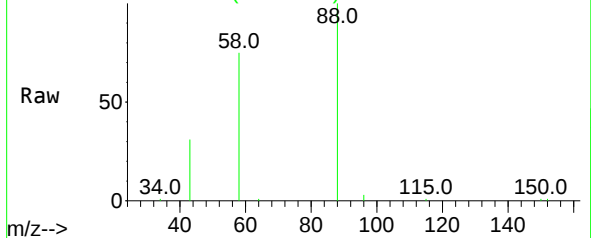

Abundance Scan 18 (2.896 min): BM032915.D\data.ms (-6)

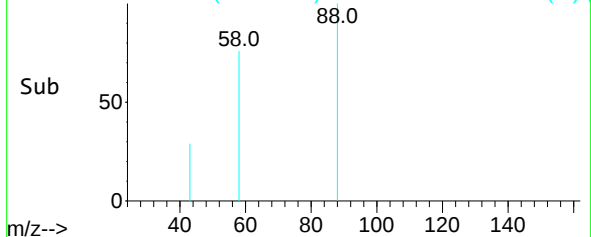

#2
1,4-Dioxane
Concen: 4.420 ng/ul
RT: 2.896 min Scan# 11
Delta R.T. -0.007 min
Lab File: BM032915.D
Acq: 09 Nov 2021 15:05

Instrument :
BNA_M
ClientSampleId :
GB862

Tgt Ion	88	Ratio	100	Lower	35.8	Upper	53.8#
43	31.1	35.8	53.8#				
58	75.2	55.8	83.8				

