

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032916.D
 Acq On : 09 Nov 2021 16:34
 Operator : CG/JU
 Sample : M4532-06DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB862DL

Quant Time: Nov 09 17:07:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.470	152	1579	0.400	ng/ul	0.00
4) Naphthalene-d8	10.244	136	5889	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.126	164	3688	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.870	188	7799	0.400	ng/ul	0.00
17) Chrysene-d12	21.058	240	6279	0.400	ng/ul	0.00
23) Perylene-d12	23.169	264	5262	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.868	96	723	0.359	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.846	152	1428	0.171	ng/ul	0.00
18) Fluoranthene-d10	18.901	212	3699	0.194	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	2.899	88	4551	2.198	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032916.D
Acq On : 09 Nov 2021 16:34
Operator : CG/JU
Sample : M4532-06DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB862DL

Quant Time: Nov 09 17:07:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

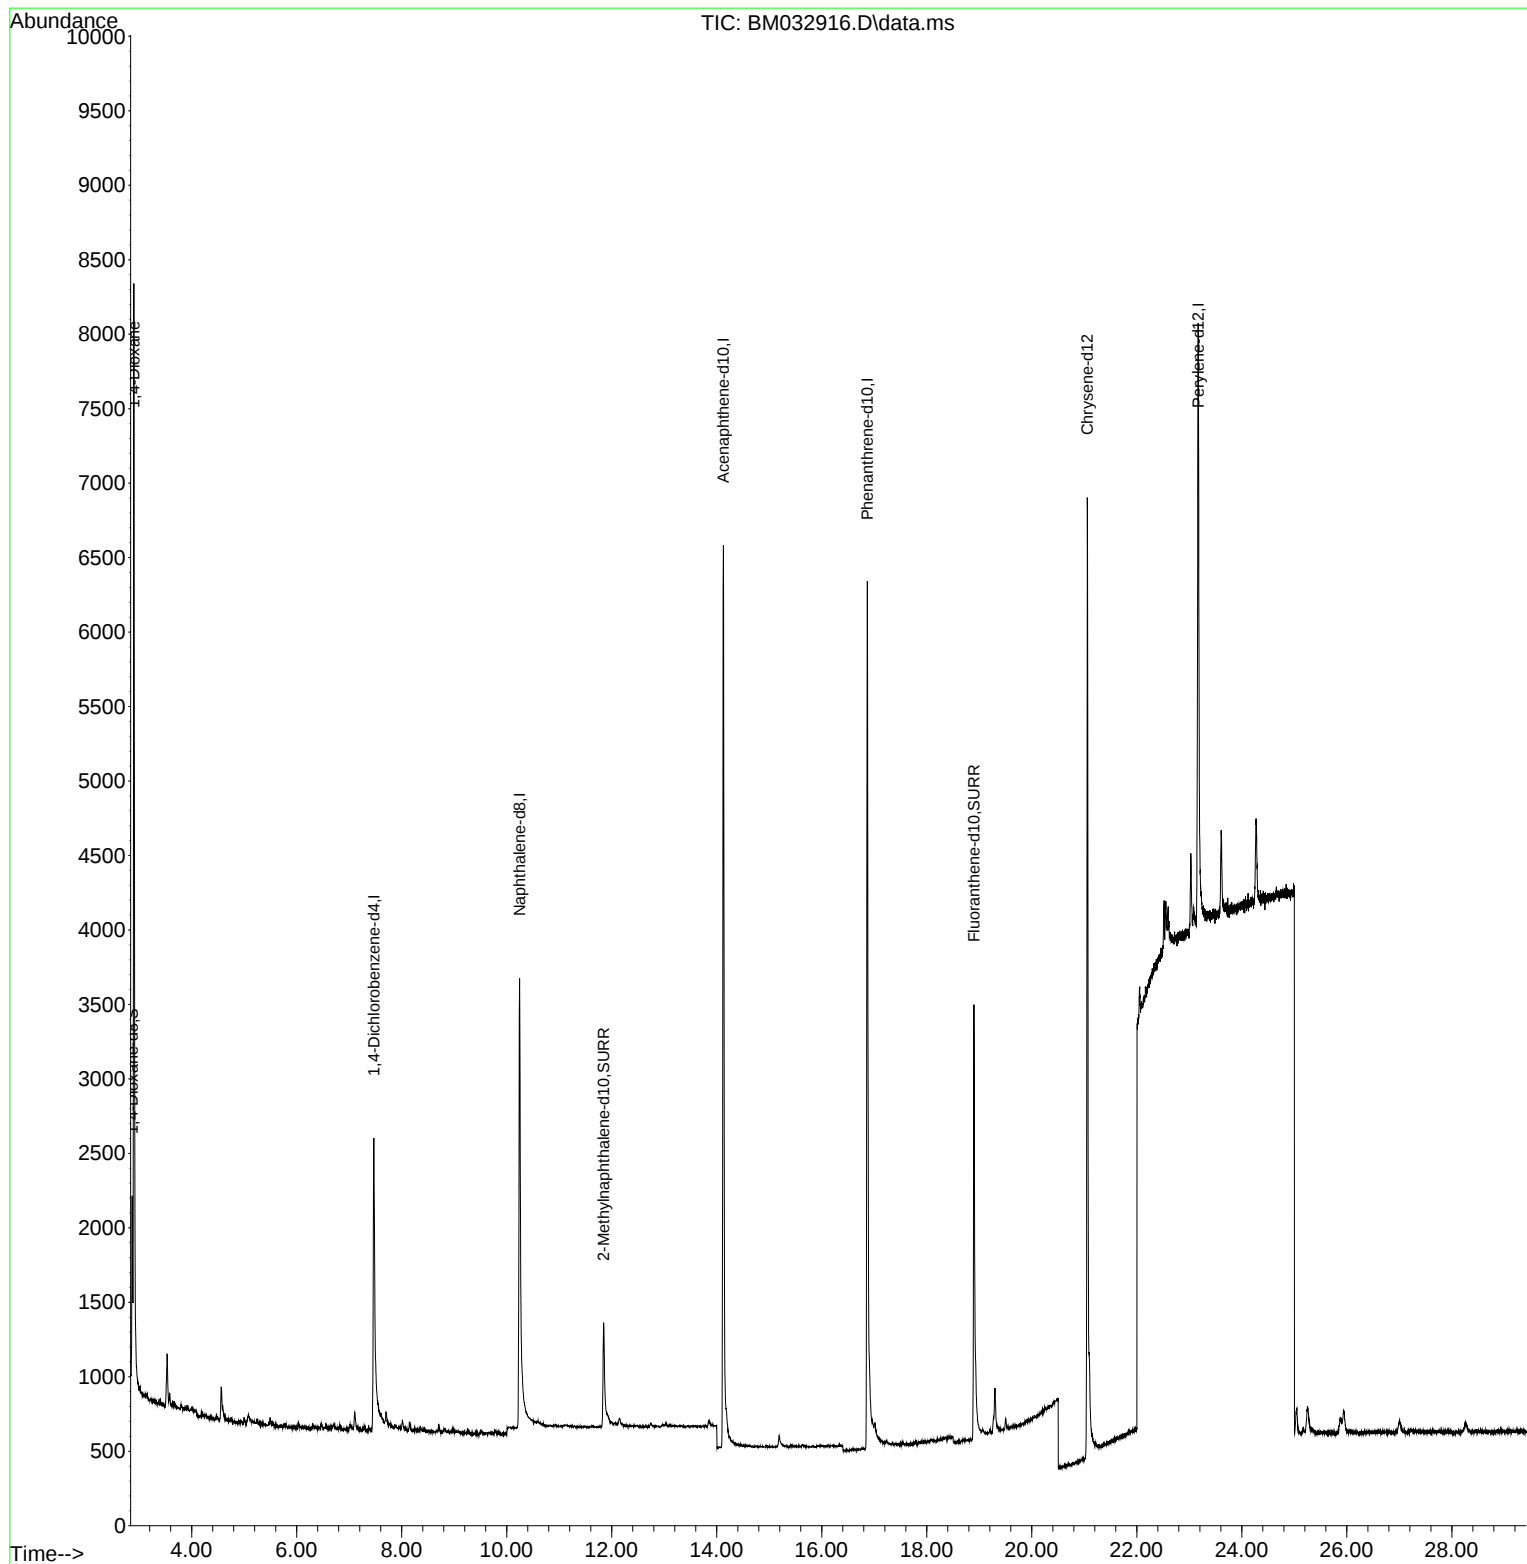

Abundance Scan 20 (2.903 min): BM032909.D\data.ms (-12)

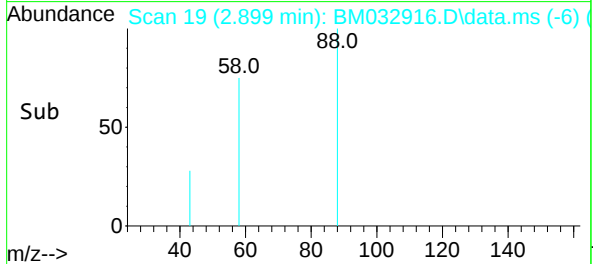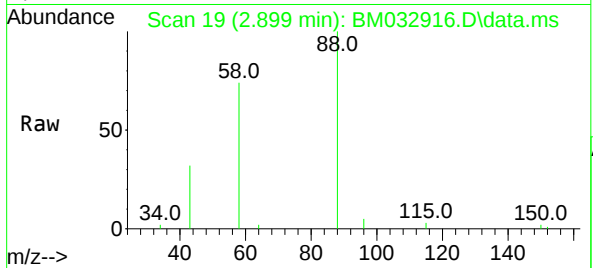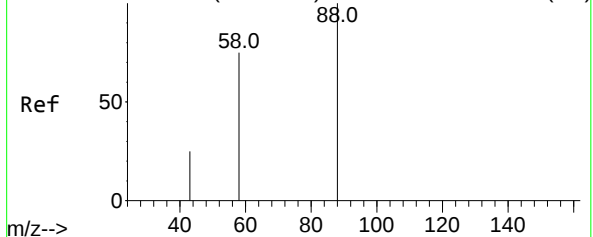

#2
1,4-Dioxane
Concen: 2.198 ng/ul
RT: 2.899 min Scan# 19
Delta R.T. -0.004 min
Lab File: BM032916.D
Acq: 09 Nov 2021 16:34

Instrument :
BNA_M
ClientSampleId :
GB862DL

Tgt Ion:	88	Resp:	4551
Ion	Ratio	Lower	Upper
88	100		
43	32.3	35.8	53.8#
58	74.0	55.8	83.8

