

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032939.D
 Acq On : 10 Nov 2021 07:00
 Operator : CG/JU
 Sample : M4532-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB8F2

Quant Time: Nov 10 08:00:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.466	152	2336	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	8376	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.121	164	5220	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.865	188	10910	0.400	ng/ul	0.00
17) Chrysene-d12	21.052	240	8945	0.400	ng/ul	0.00
23) Perylene-d12	23.159	264	8745	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.860	96	12525	4.199	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.840	152	3949	0.332	ng/ul	0.00
18) Fluoranthene-d10	18.892	212	12629	0.466	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	2.898	88	84	0.027	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032939.D
Acq On : 10 Nov 2021 07:00
Operator : CG/JU
Sample : M4532-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB8F2


Quant Time: Nov 10 08:00:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

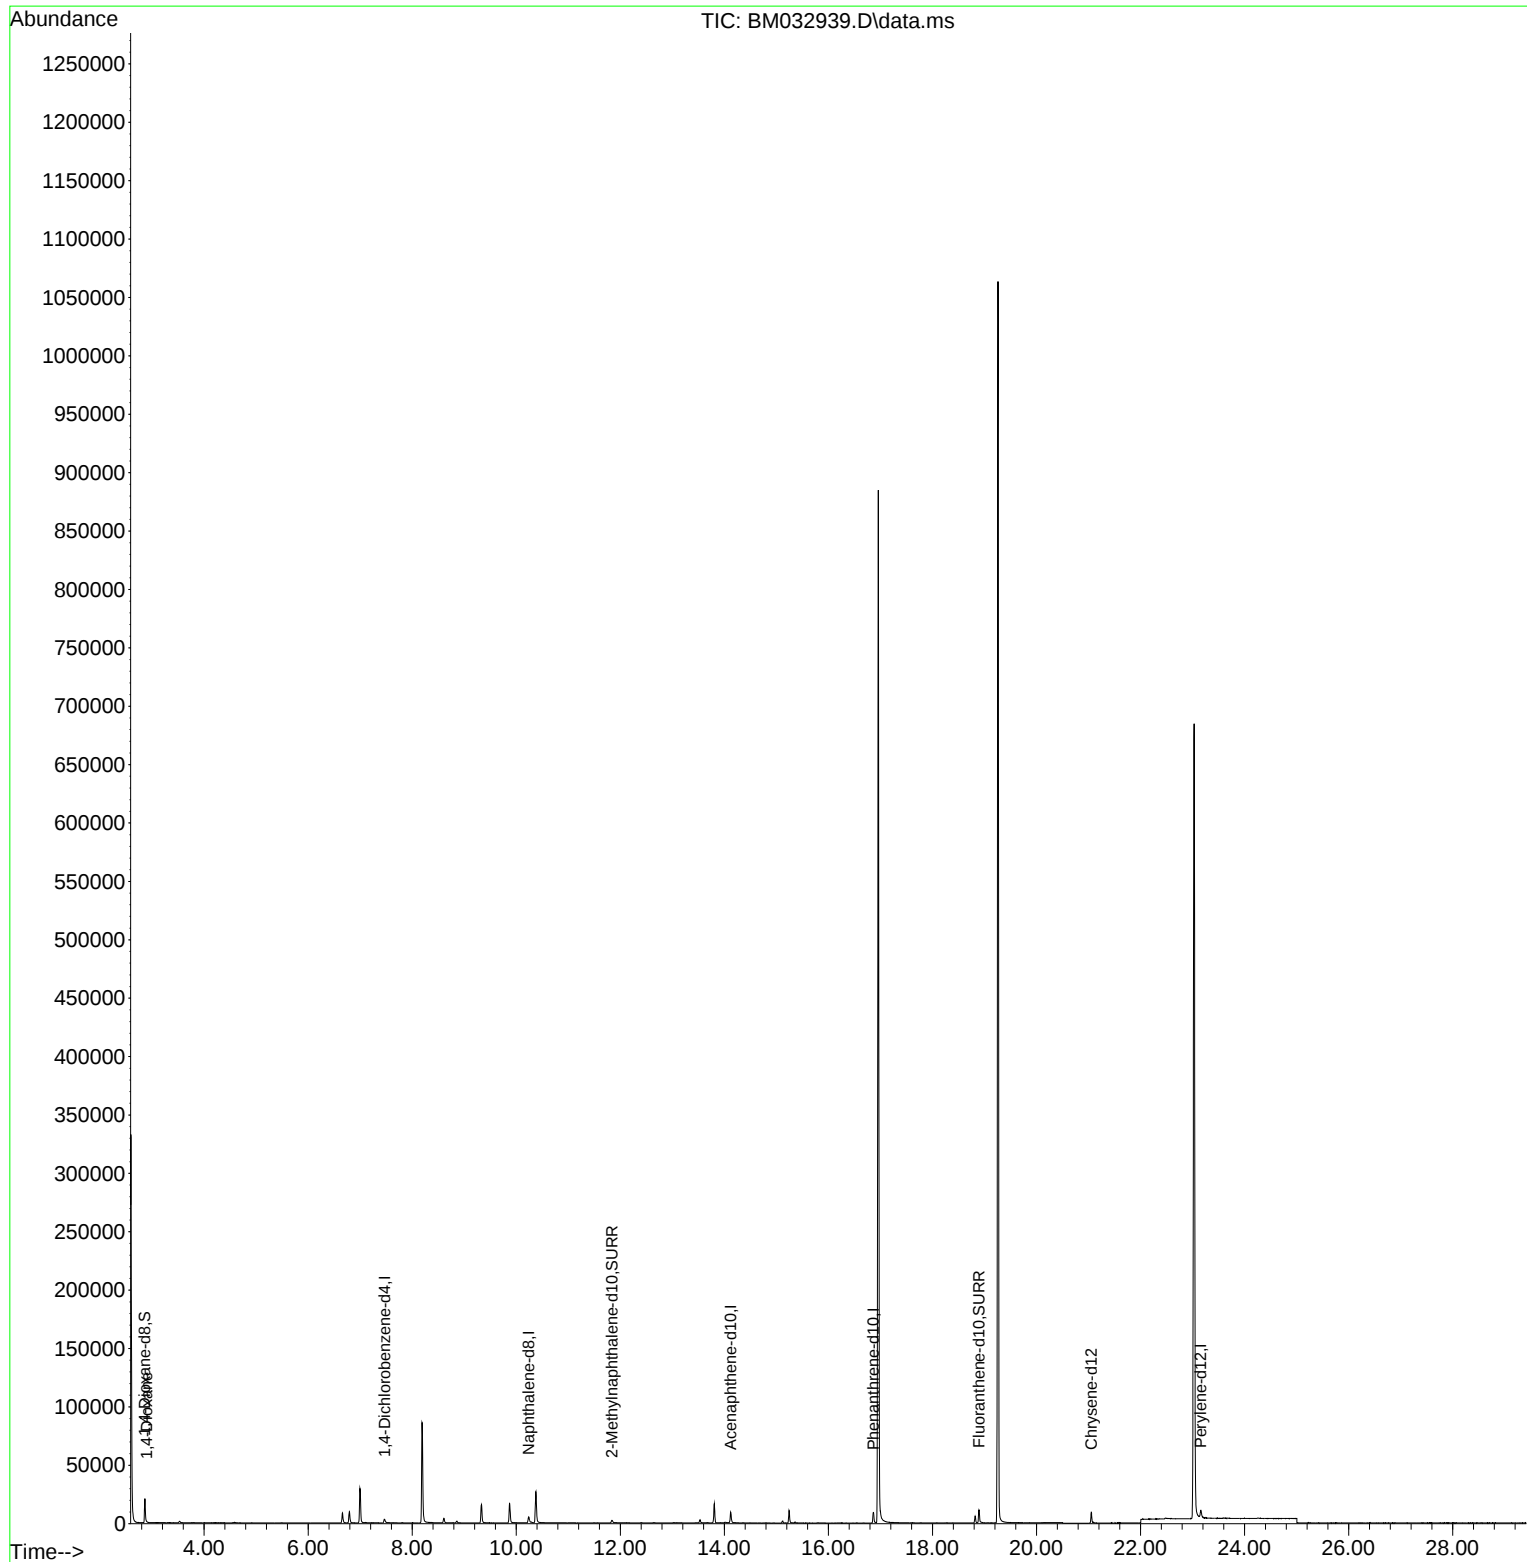

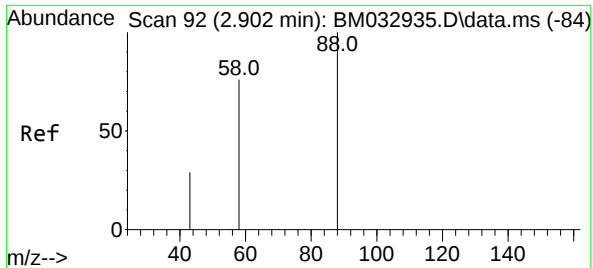

#2
 1,4-Dioxane
 Concen: 0.027 ng/ul
 RT: 2.898 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM032939.D
 Acq: 10 Nov 2021 07:00

Instrument :
 BNA_M
 ClientSampleId :
 GB8F2

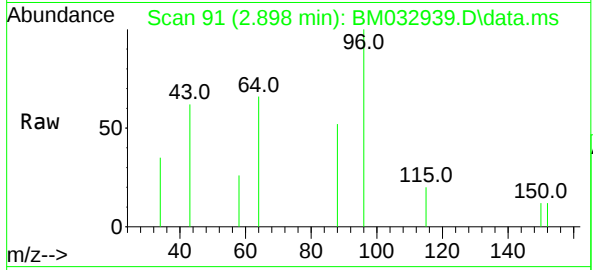

Tgt Ion: 88 Resp: 84

Ion	Ratio	Lower	Upper
88	100		
43	120.5	35.8	53.8#
58	50.4	55.8	83.8#

