

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032952.D
 Acq On : 10 Nov 2021 14:53
 Operator : CG/JU
 Sample : M4400-05
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG334

Quant Time: Nov 10 15:24:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.462	152	2132	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	7875	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.121	164	4807	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.862	188	10272	0.400	ng/ul	0.00
17) Chrysene-d12	21.052	240	8782	0.400	ng/ul	0.00
23) Perylene-d12	23.159	264	8655	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.860	96	12139	4.459	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.840	152	3059	0.274	ng/ul	0.00
18) Fluoranthene-d10	18.892	212	9834	0.369	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.539	266	67	0.025	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032952.D
Acq On : 10 Nov 2021 14:53
Operator : CG/JU
Sample : M4400-05
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG334


Quant Time: Nov 10 15:24:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

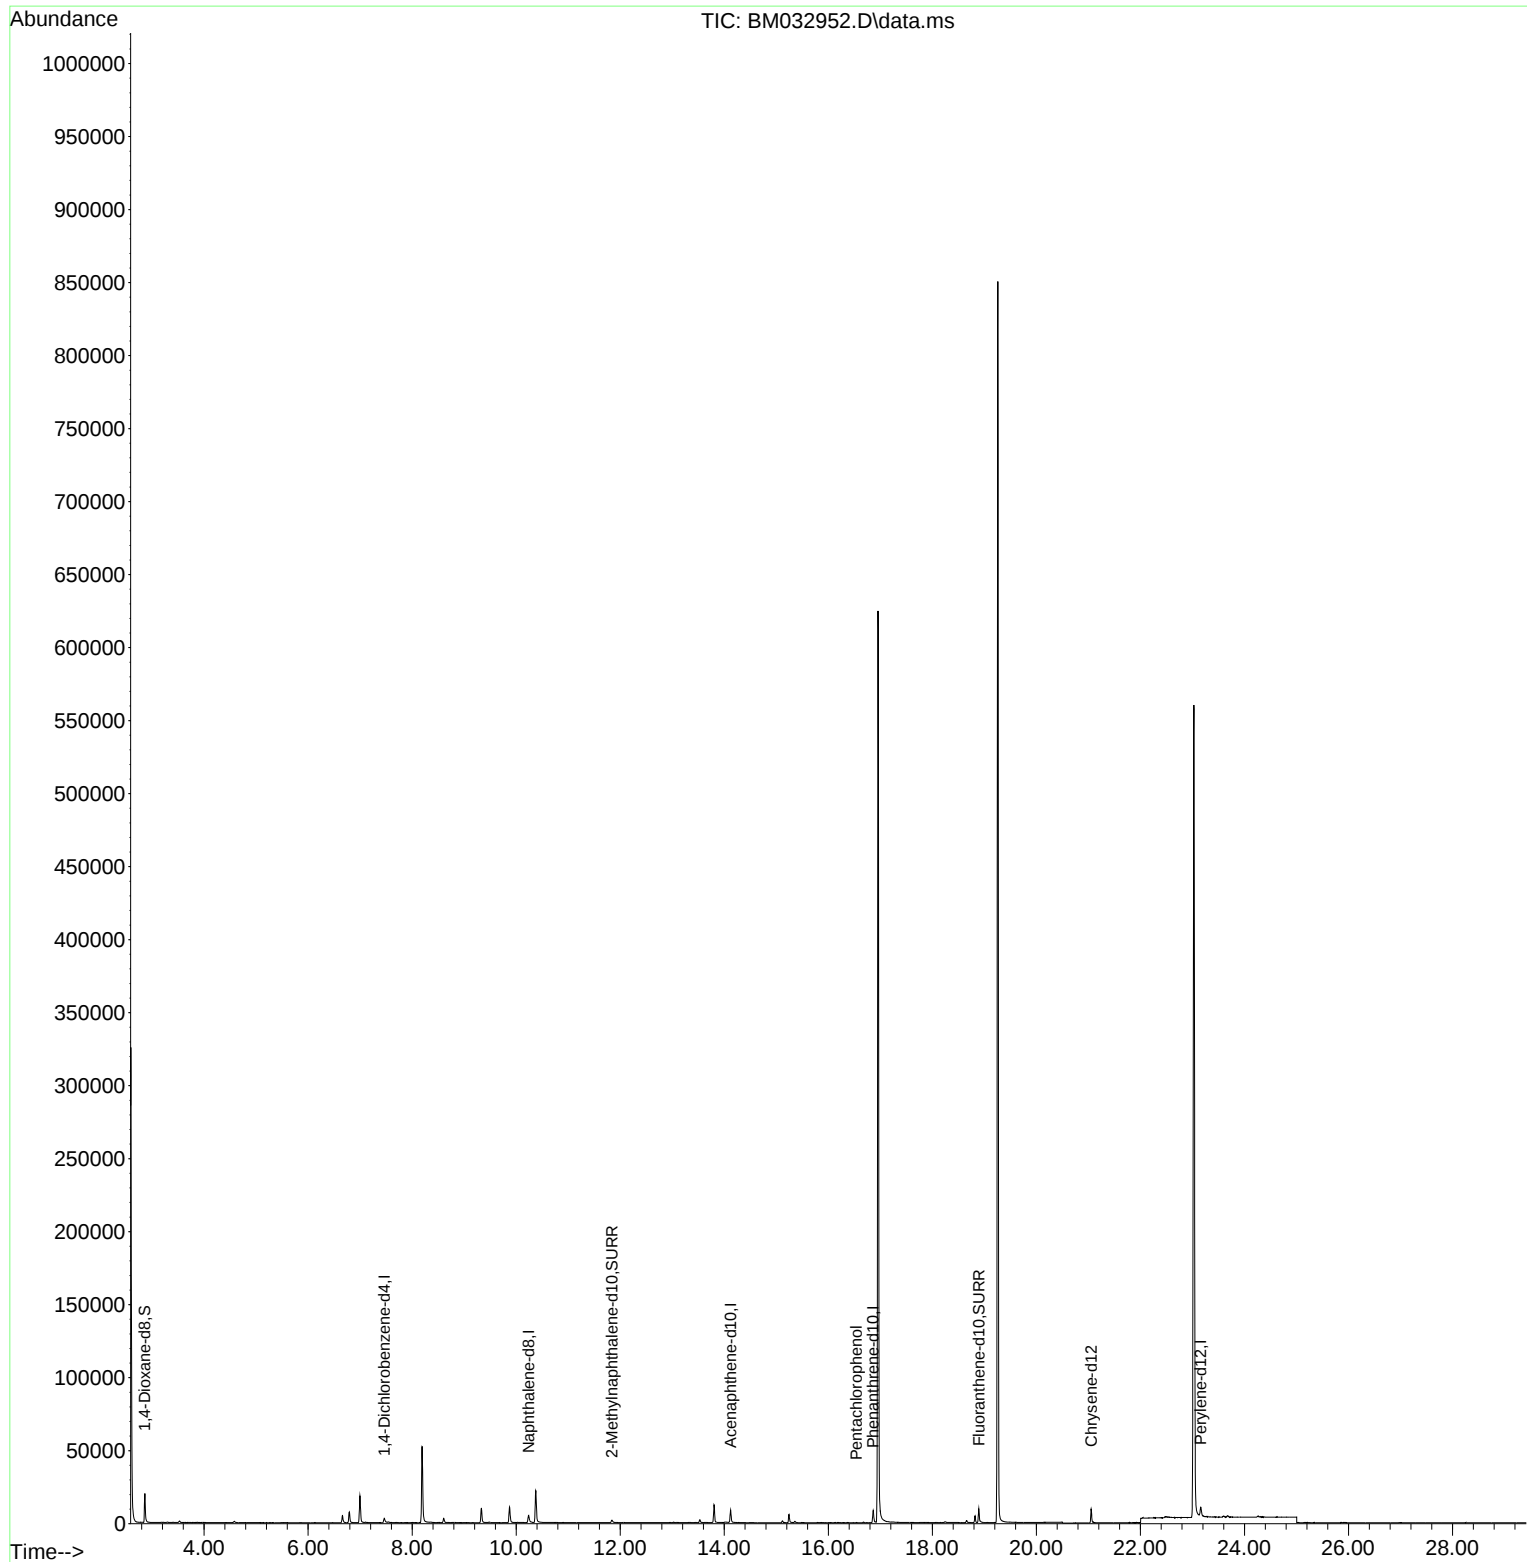

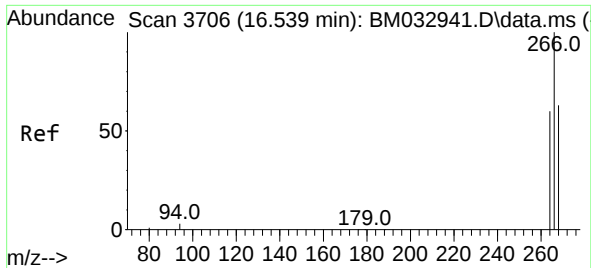

#14
 Pentachlorophenol
 Concen: 0.025 ng/ul
 RT: 16.539 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BM032952.D
 Acq: 10 Nov 2021 14:53

Instrument :
 BNA_M
 ClientSampleId :
 BG334

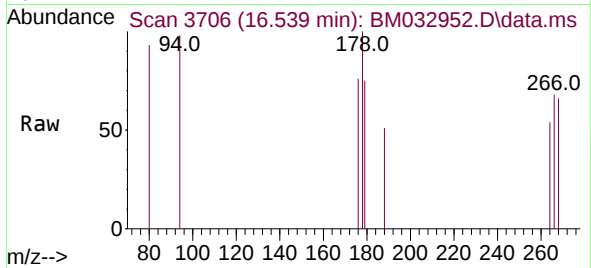

Tgt Ion:	266	Resp:	67
Ion	Ratio	Lower	Upper
266	100		
264	59.7	51.2	76.8
268	61.2	52.9	79.3

