

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032956.D
 Acq On : 10 Nov 2021 17:21
 Operator : CG/JU
 Sample : M4401-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG333

Quant Time: Nov 10 17:51:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.462	152	2140	0.400	ng/ul	0.00
4) Naphthalene-d8	10.235	136	7768	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.118	164	4711	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.862	188	9863	0.400	ng/ul	0.00
17) Chrysene-d12	21.052	240	7850	0.400	ng/ul	0.00
23) Perylene-d12	23.161	264	7225	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.860	96	10861	3.974	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.836	152	3409	0.309	ng/ul	0.00
18) Fluoranthene-d10	18.892	212	9950	0.418	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.543	266	68	0.026	ng/ul	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032956.D
Acq On : 10 Nov 2021 17:21
Operator : CG/JU
Sample : M4401-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG333

Quant Time: Nov 10 17:51:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

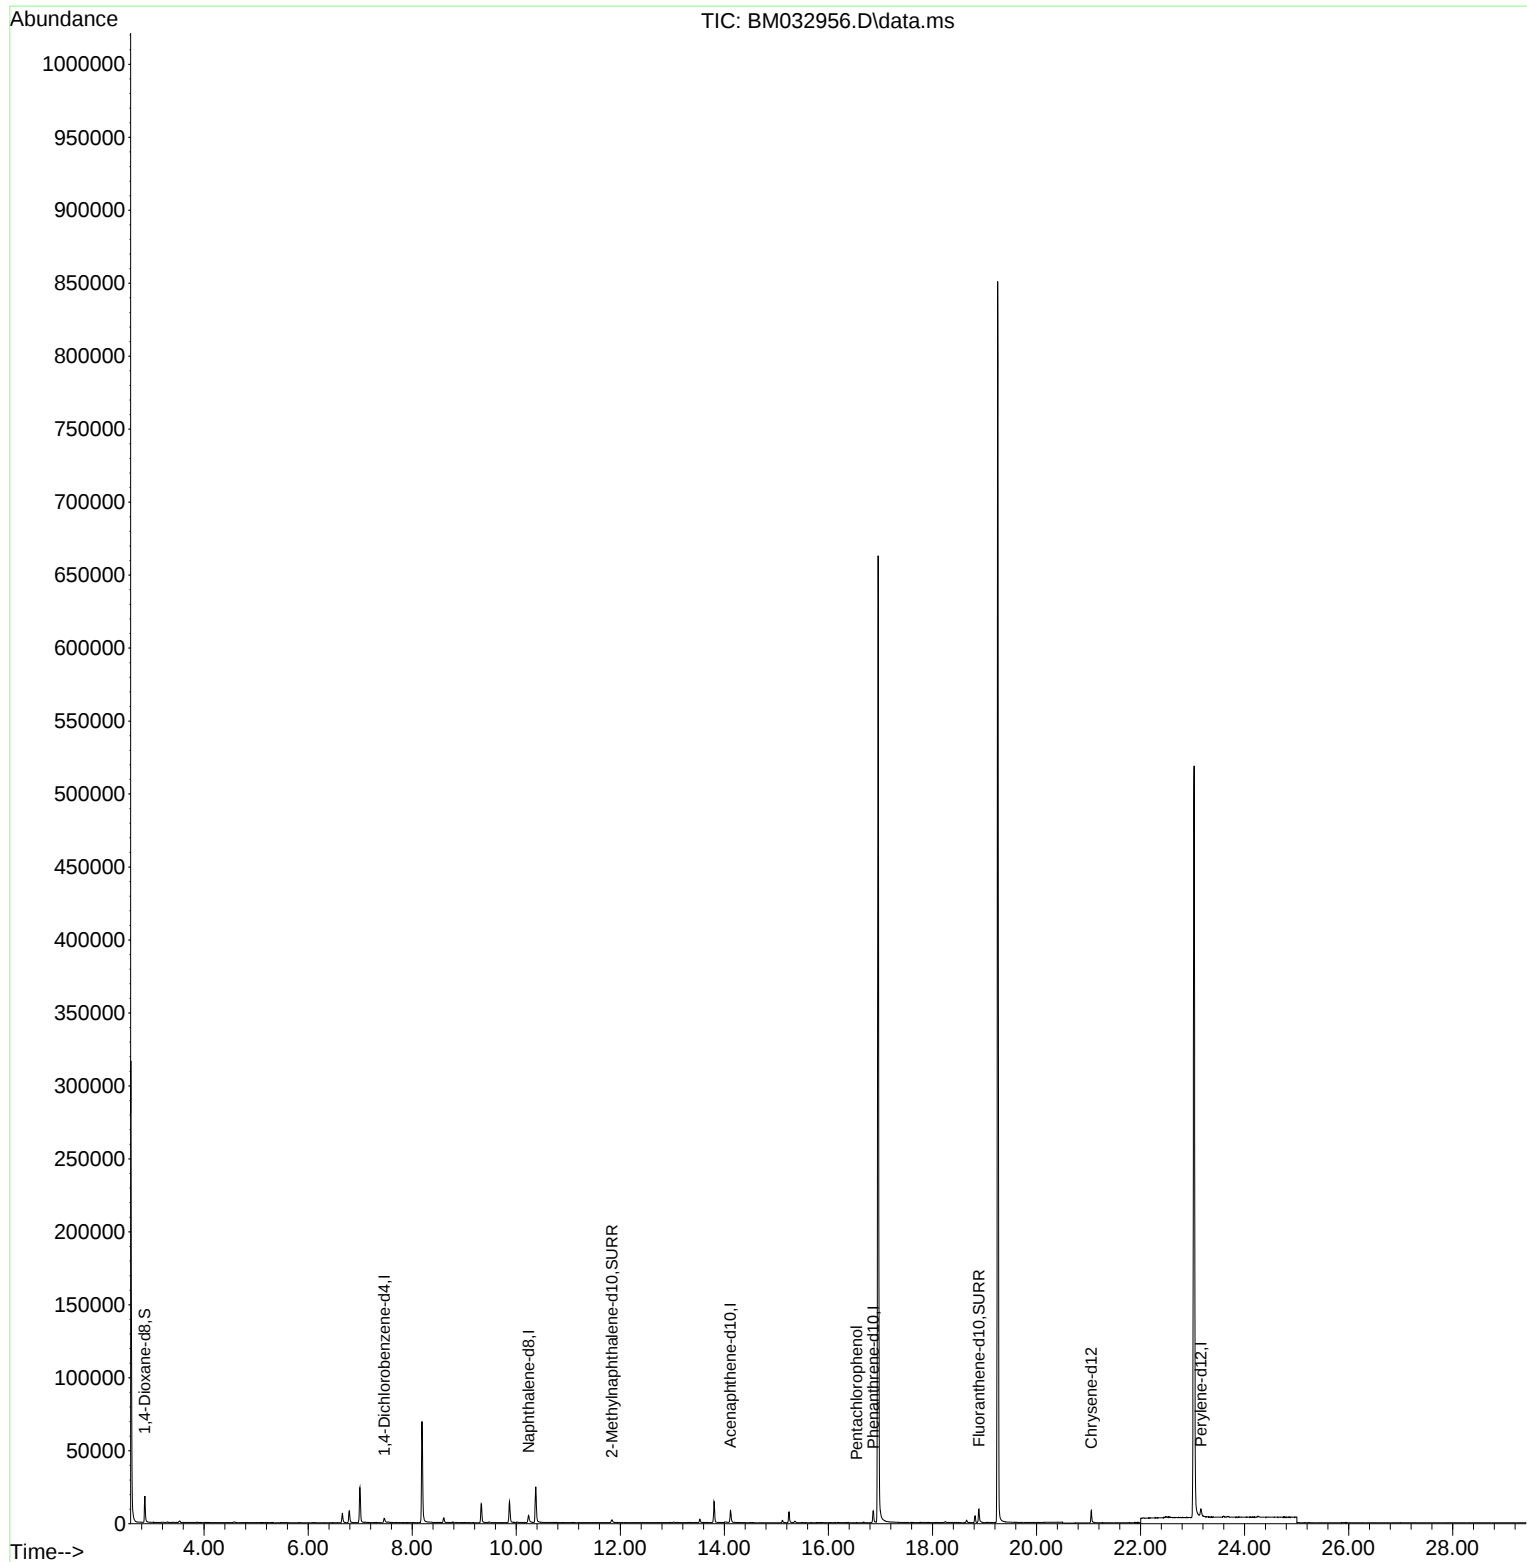

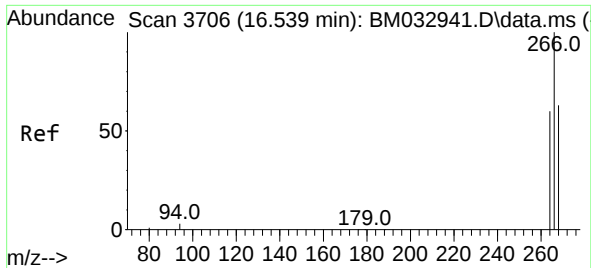

#14
 Pentachlorophenol
 Concen: 0.026 ng/ul
 RT: 16.543 min Scan# 31
 Delta R.T. -0.001 min
 Lab File: BM032956.D
 Acq: 10 Nov 2021 17:21

Instrument :
 BNA_M
 ClientSampleId :
 BG333

Tgt Ion:	266	Resp:	68
Ion	Ratio	Lower	Upper
266	100		
264	54.4	51.2	76.8
268	60.3	52.9	79.3

