

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032974.D
 Acq On : 11 Nov 2021 04:10
 Operator : CG/JU
 Sample : M4400-08
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG343

Quant Time: Nov 11 09:34:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	2667	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.235	136	9899	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.117	164	6087	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.858	188	13057	0.400	ng/ul	0.00
17) Chrysene-d12	21.049	240	10814	0.400	ng/ul	0.00
23) Perylene-d12	23.154	264	10127	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.857	96	14912	4.379	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.831	152	4166	0.296	ng/ul	0.00
18) Fluoranthene-d10	18.888	212	12295	0.375	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.532	266	69	0.020	ng/ul	94
15) Phenanthrene	16.900	178	1001	0.023	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032974.D
Acq On : 11 Nov 2021 04:10
Operator : CG/JU
Sample : M4400-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG343

Quant Time: Nov 11 09:34:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration




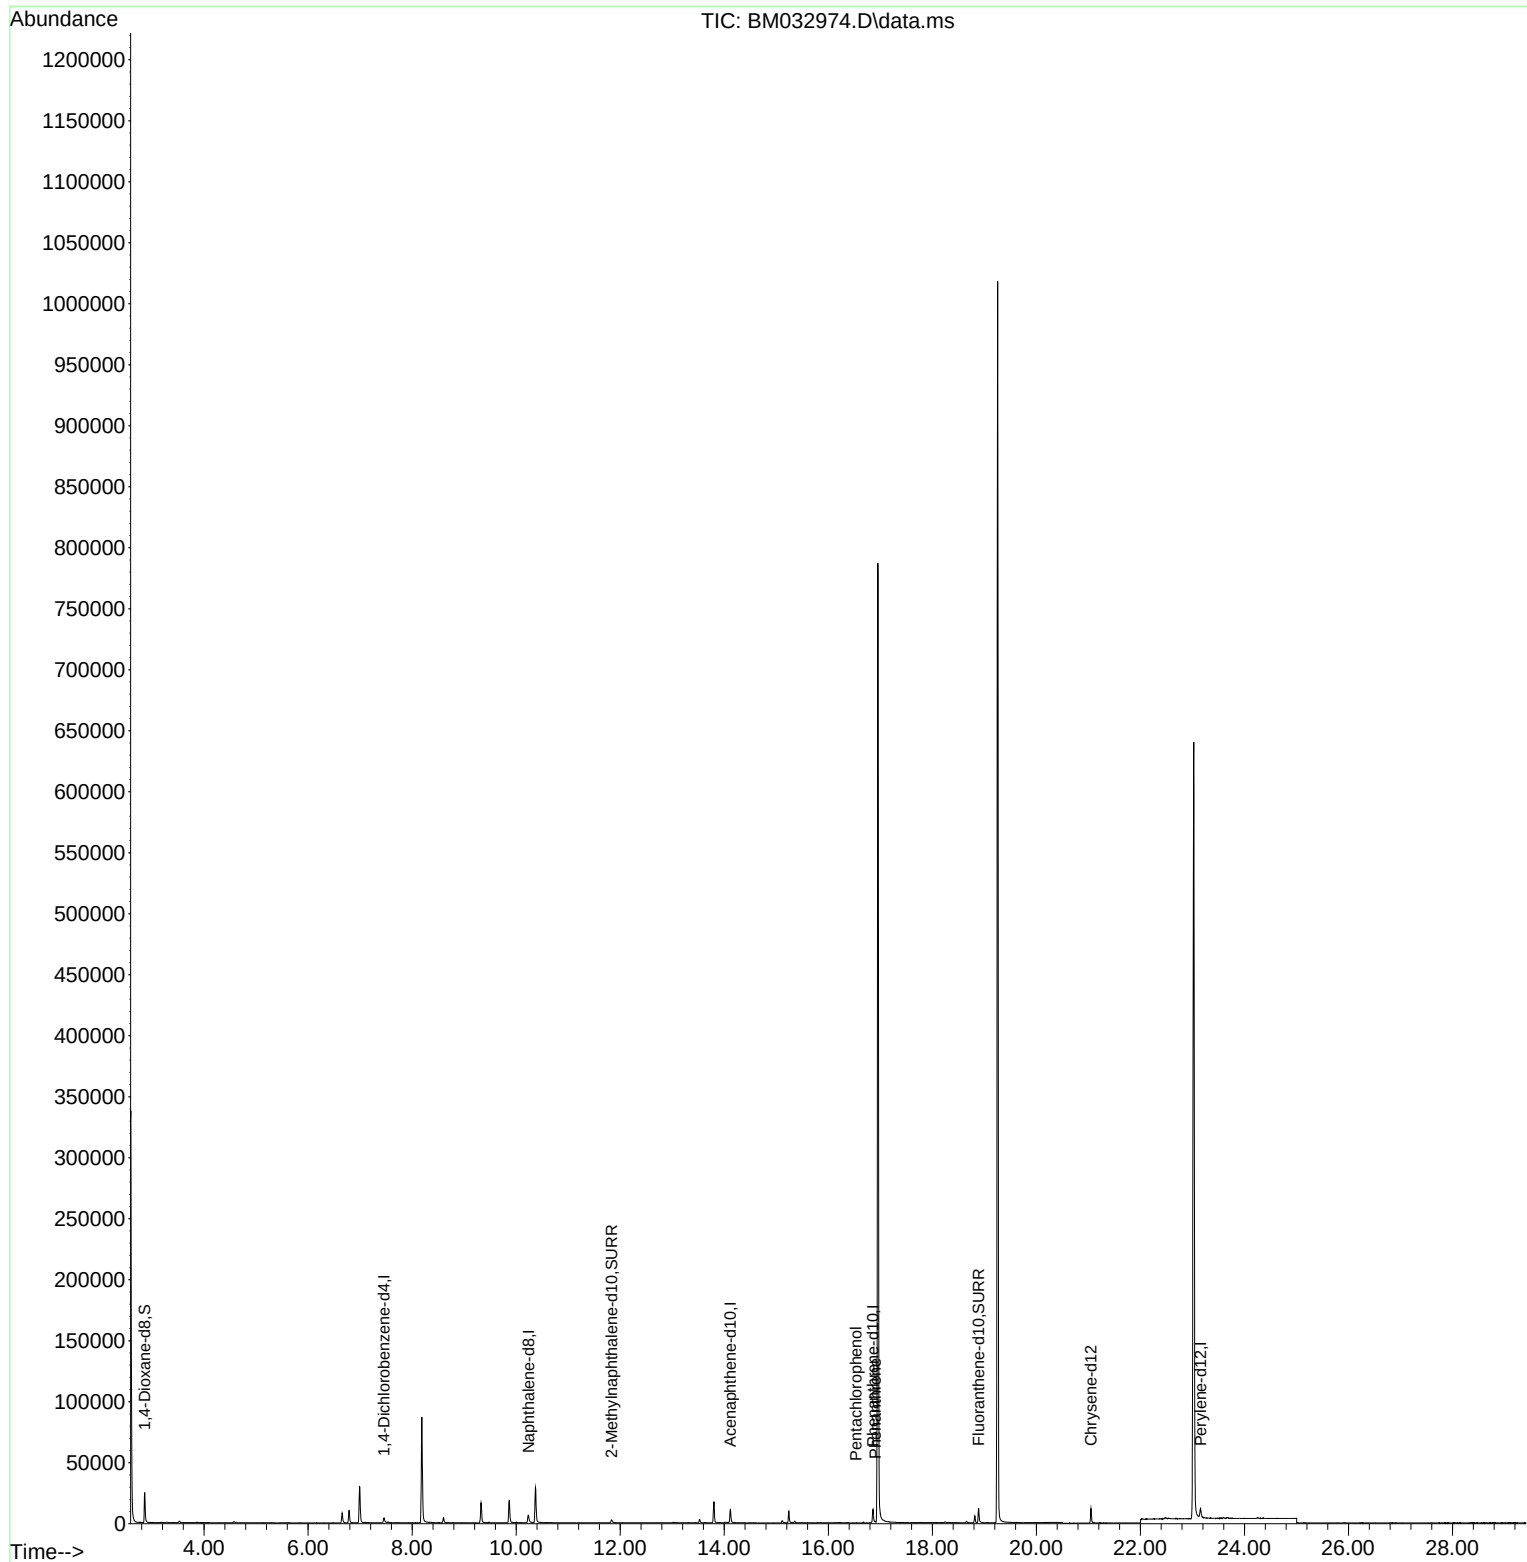


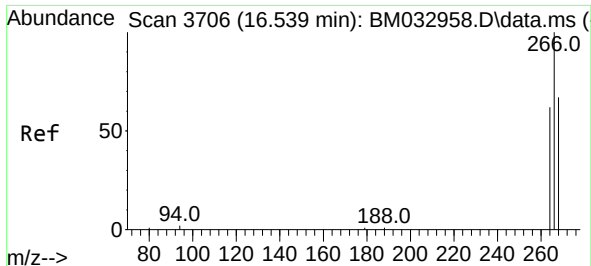

#14
 Pentachlorophenol
 Concen: 0.020 ng/ul
 RT: 16.532 min Scan# 31
 Delta R.T. -0.011 min
 Lab File: BM032974.D
 Acq: 11 Nov 2021 04:10

Instrument :
 BNA_M
 ClientSampleId :
 BG343

Tgt Ion:266	Resp:	69
Ion Ratio	Lower	Upper
266	100	
264	59.4	51.2 76.8
268	60.9	52.9 79.3

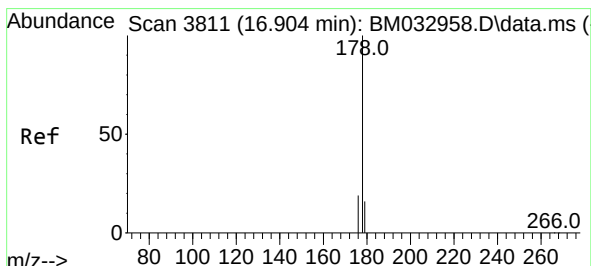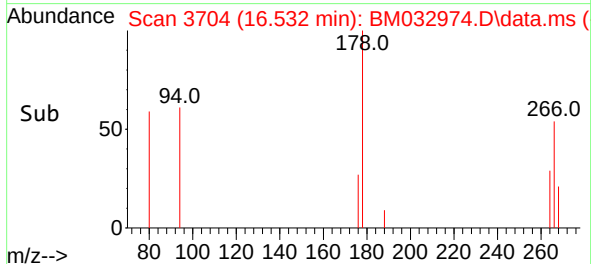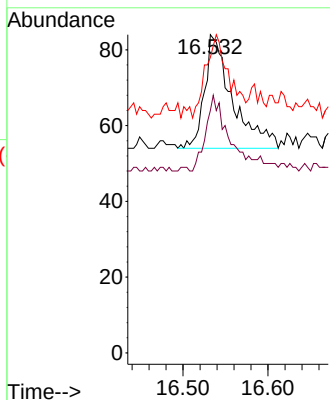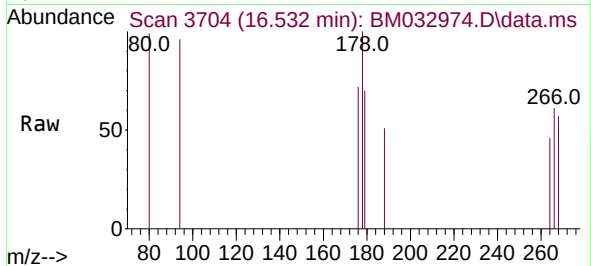

#15
 Phenanthrene
 Concen: 0.023 ng/ul
 RT: 16.900 min Scan# 3810
 Delta R.T. -0.008 min
 Lab File: BM032974.D
 Acq: 11 Nov 2021 04:10

Tgt Ion:178	Resp:	1001
Ion Ratio	Lower	Upper
178	100	
179	26.1	12.9 19.3#
176	25.8	16.0 24.0#

