

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032980.D
 Acq On : 11 Nov 2021 08:20
 Operator : CG/JU
 Sample : M4400-07
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG338

Quant Time: Nov 11 09:38:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	2609	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.230	136	9523	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.114	164	5788	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	16.858	188	12355	0.400	ng/ul	0.00
17) Chrysene-d12	21.049	240	9818	0.400	ng/ul	0.00
23) Perylene-d12	23.156	264	9136	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.857	96	13866	4.162	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.831	152	3751	0.277	ng/ul	0.00
18) Fluoranthene-d10	18.888	212	10959	0.368	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.536	266	85	0.026	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032980.D
Acq On : 11 Nov 2021 08:20
Operator : CG/JU
Sample : M4400-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG338

Quant Time: Nov 11 09:38:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

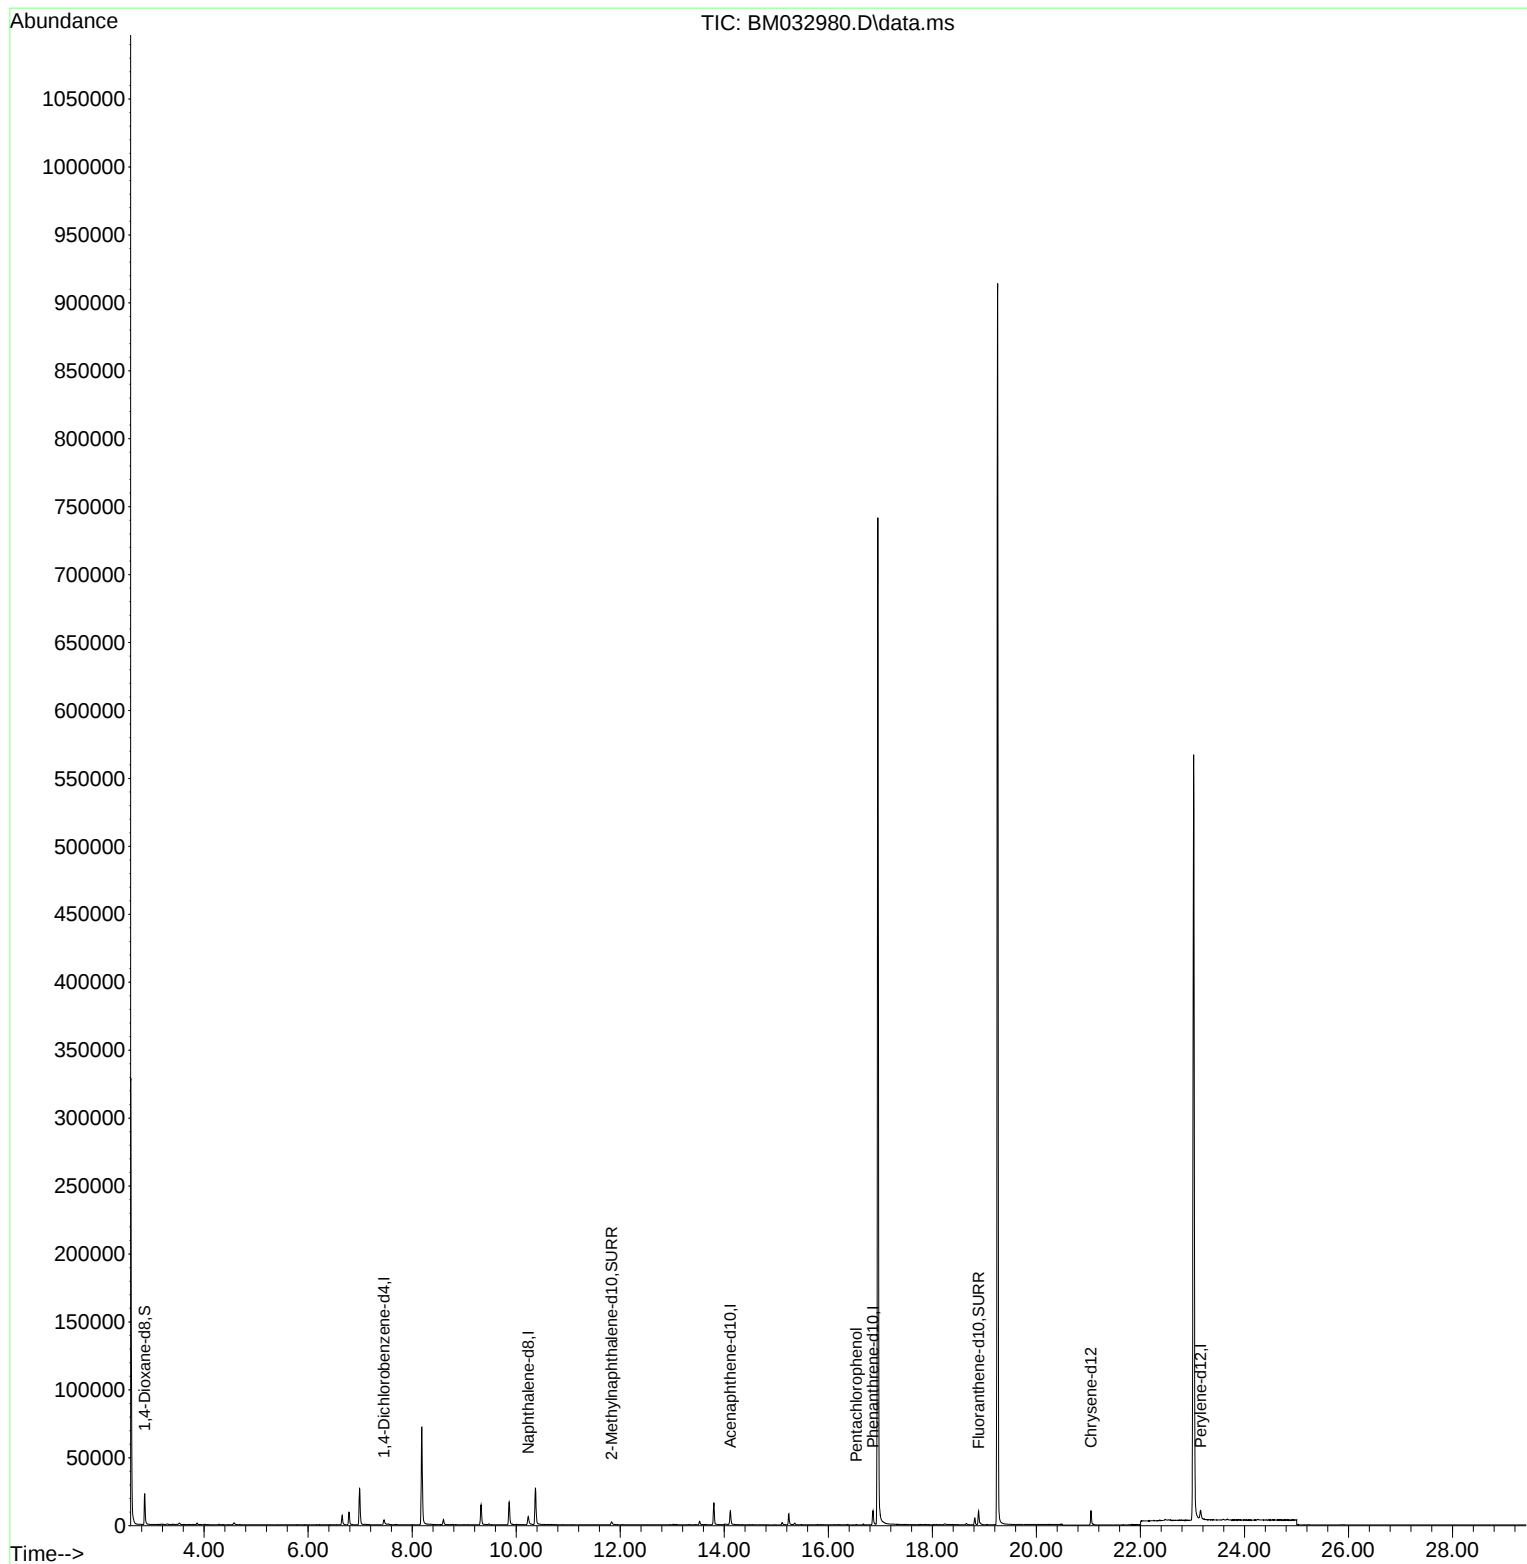

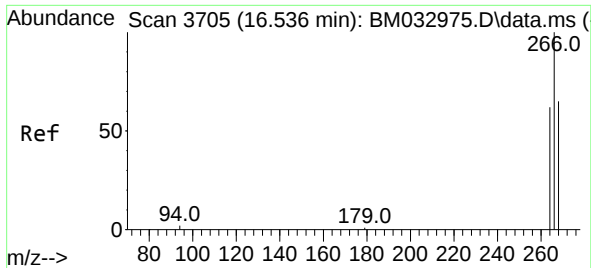

#14

Pentachlorophenol

Concen: 0.026 ng/ul

RT: 16.536 min Scan# 31

Delta R.T. -0.008 min

Lab File: BM032980.D


Acq: 11 Nov 2021 08:20

Instrument :

BNA_M

ClientSampleId :

BG338

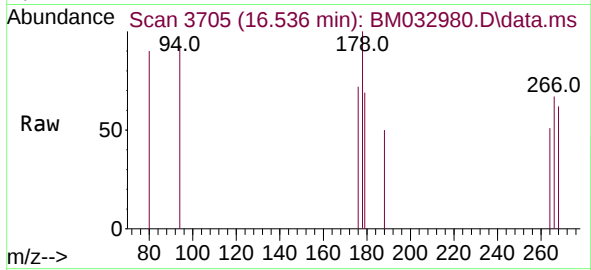

Tgt Ion:266 Resp: 85

Ion Ratio Lower Upper

266 100

264 55.3 51.2 76.8

268 62.4 52.9 79.3

