

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032983.D
 Acq On : 11 Nov 2021 10:07
 Operator : CG/JU
 Sample : M4401-08
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG345

Quant Time: Nov 11 10:45:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	2635	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.230	136	9914	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.114	164	6031	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	16.858	188	12800	0.400	ng/ul	0.00
17) Chrysene-d12	21.047	240	9776	0.400	ng/ul	0.00
23) Perylene-d12	23.151	264	8765	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.857	96	14251	4.235	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.831	152	4523	0.321	ng/ul	0.00
18) Fluoranthene-d10	18.888	212	12541	0.423	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.897	178	3327	0.078	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032983.D
Acq On : 11 Nov 2021 10:07
Operator : CG/JU
Sample : M4401-08
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG345


Quant Time: Nov 11 10:45:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

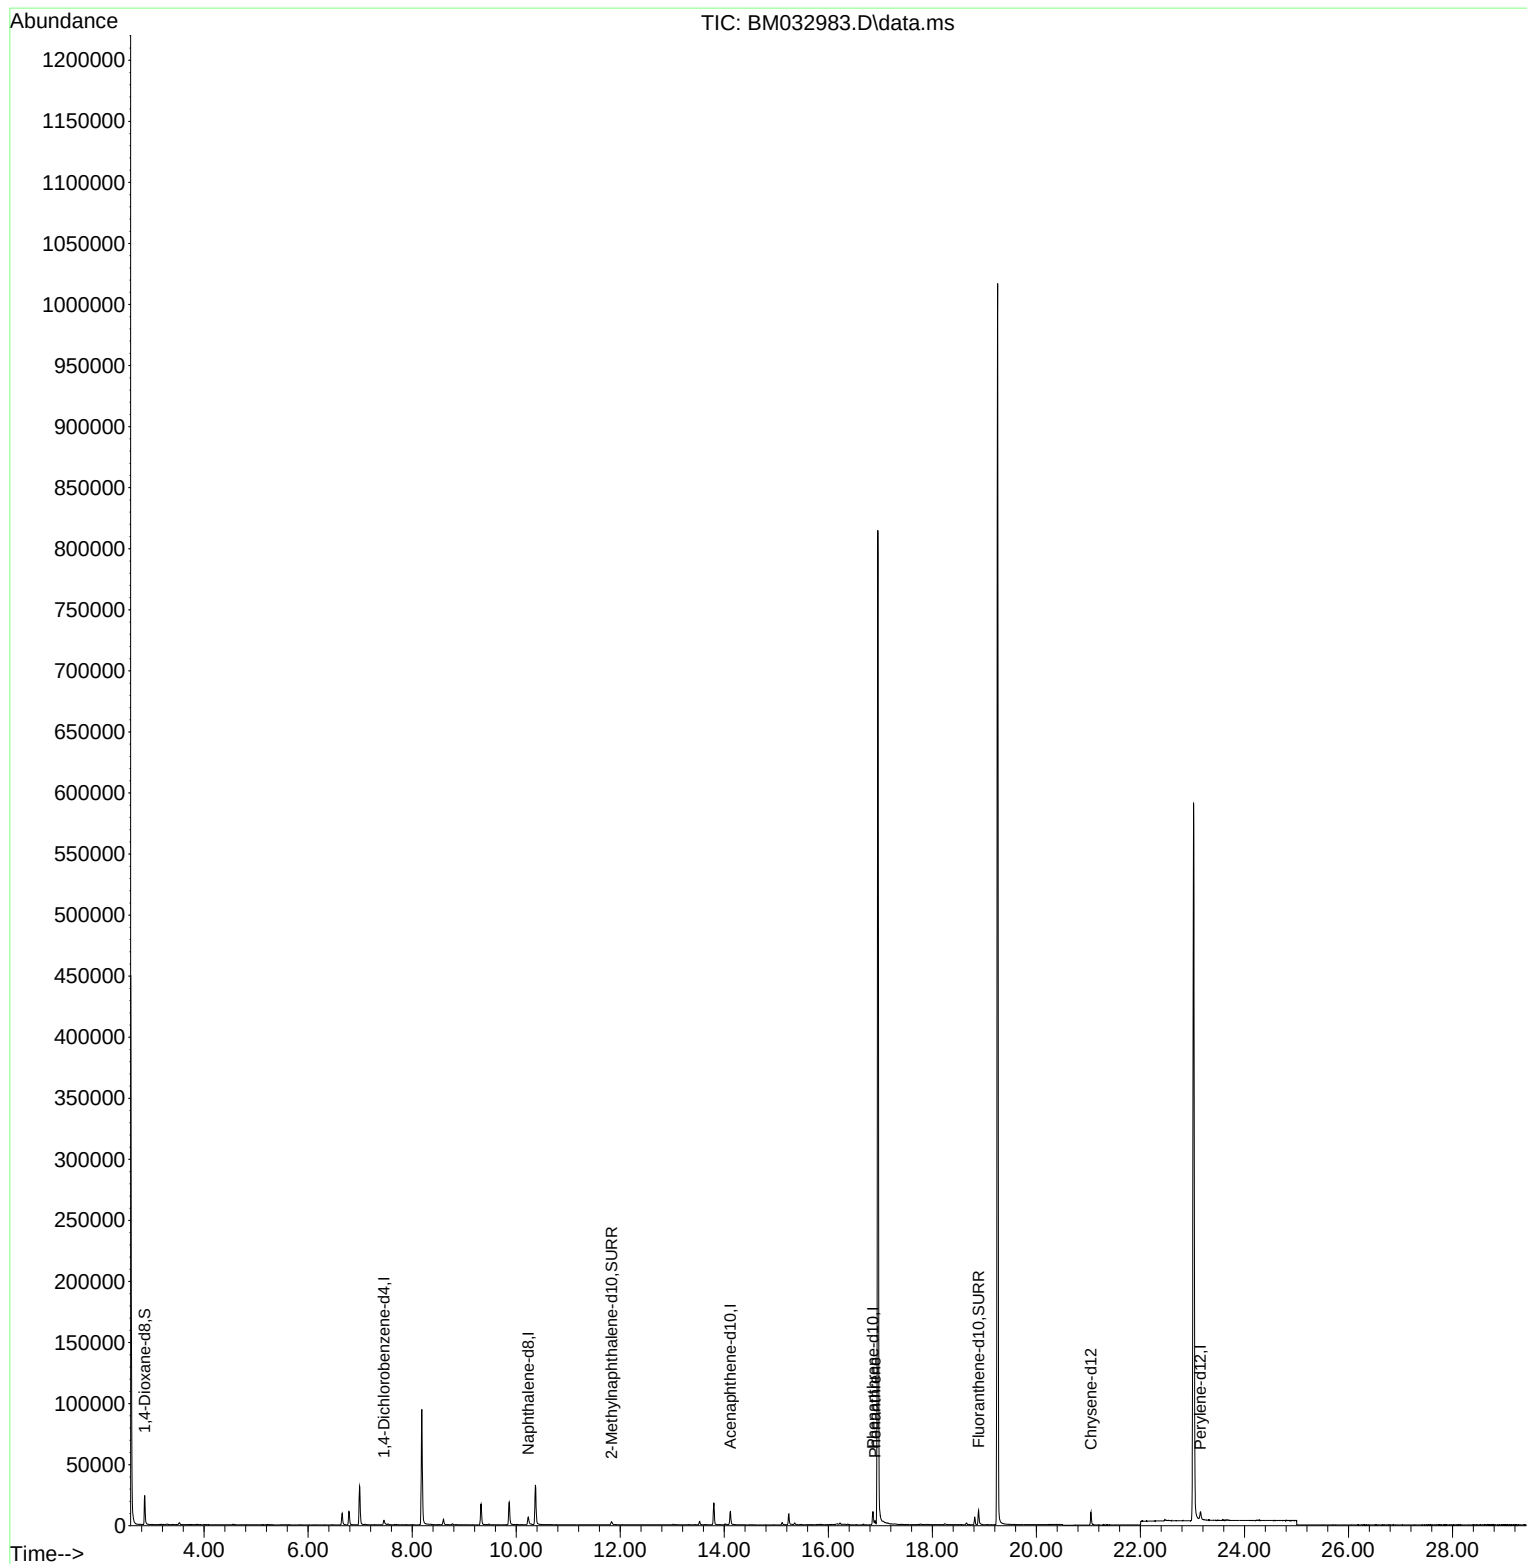

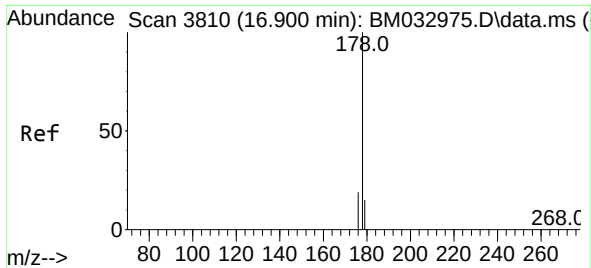

#15
 Phenanthrene
 Concen: 0.078 ng/ul
 RT: 16.897 min Scan# 31
 Delta R.T. -0.011 min
 Lab File: BM032983.D
 Acq: 11 Nov 2021 10:07

Instrument :
 BNA_M
 ClientSampleId :
 BG345

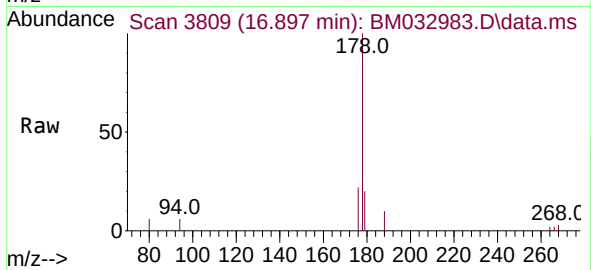

Tgt Ion:178 Resp: 3327
 Ion Ratio Lower Upper
 178 100
 179 19.8 12.9 19.3#
 176 22.1 16.0 24.0

