

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032986.D
 Acq On : 11 Nov 2021 11:55
 Operator : CG/JU
 Sample : M4401-05
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG338

Quant Time: Nov 11 12:33:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 13:31:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.455	152	2691	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.230	136	10027	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.114	164	6138	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.858	188	12802	0.400	ng/ul	0.00
17) Chrysene-d12	21.049	240	9541	0.400	ng/ul	0.00
23) Perylene-d12	23.154	264	8261	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.857	96	10666	3.104	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.831	152	3996	0.281	ng/ul	0.00
18) Fluoranthene-d10	18.888	212	11072	0.383	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.539	266	89	0.027	ng/ul	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032986.D
Acq On : 11 Nov 2021 11:55
Operator : CG/JU
Sample : M4401-05
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG338


Quant Time: Nov 11 12:33:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 13:31:56 2021
Response via : Initial Calibration

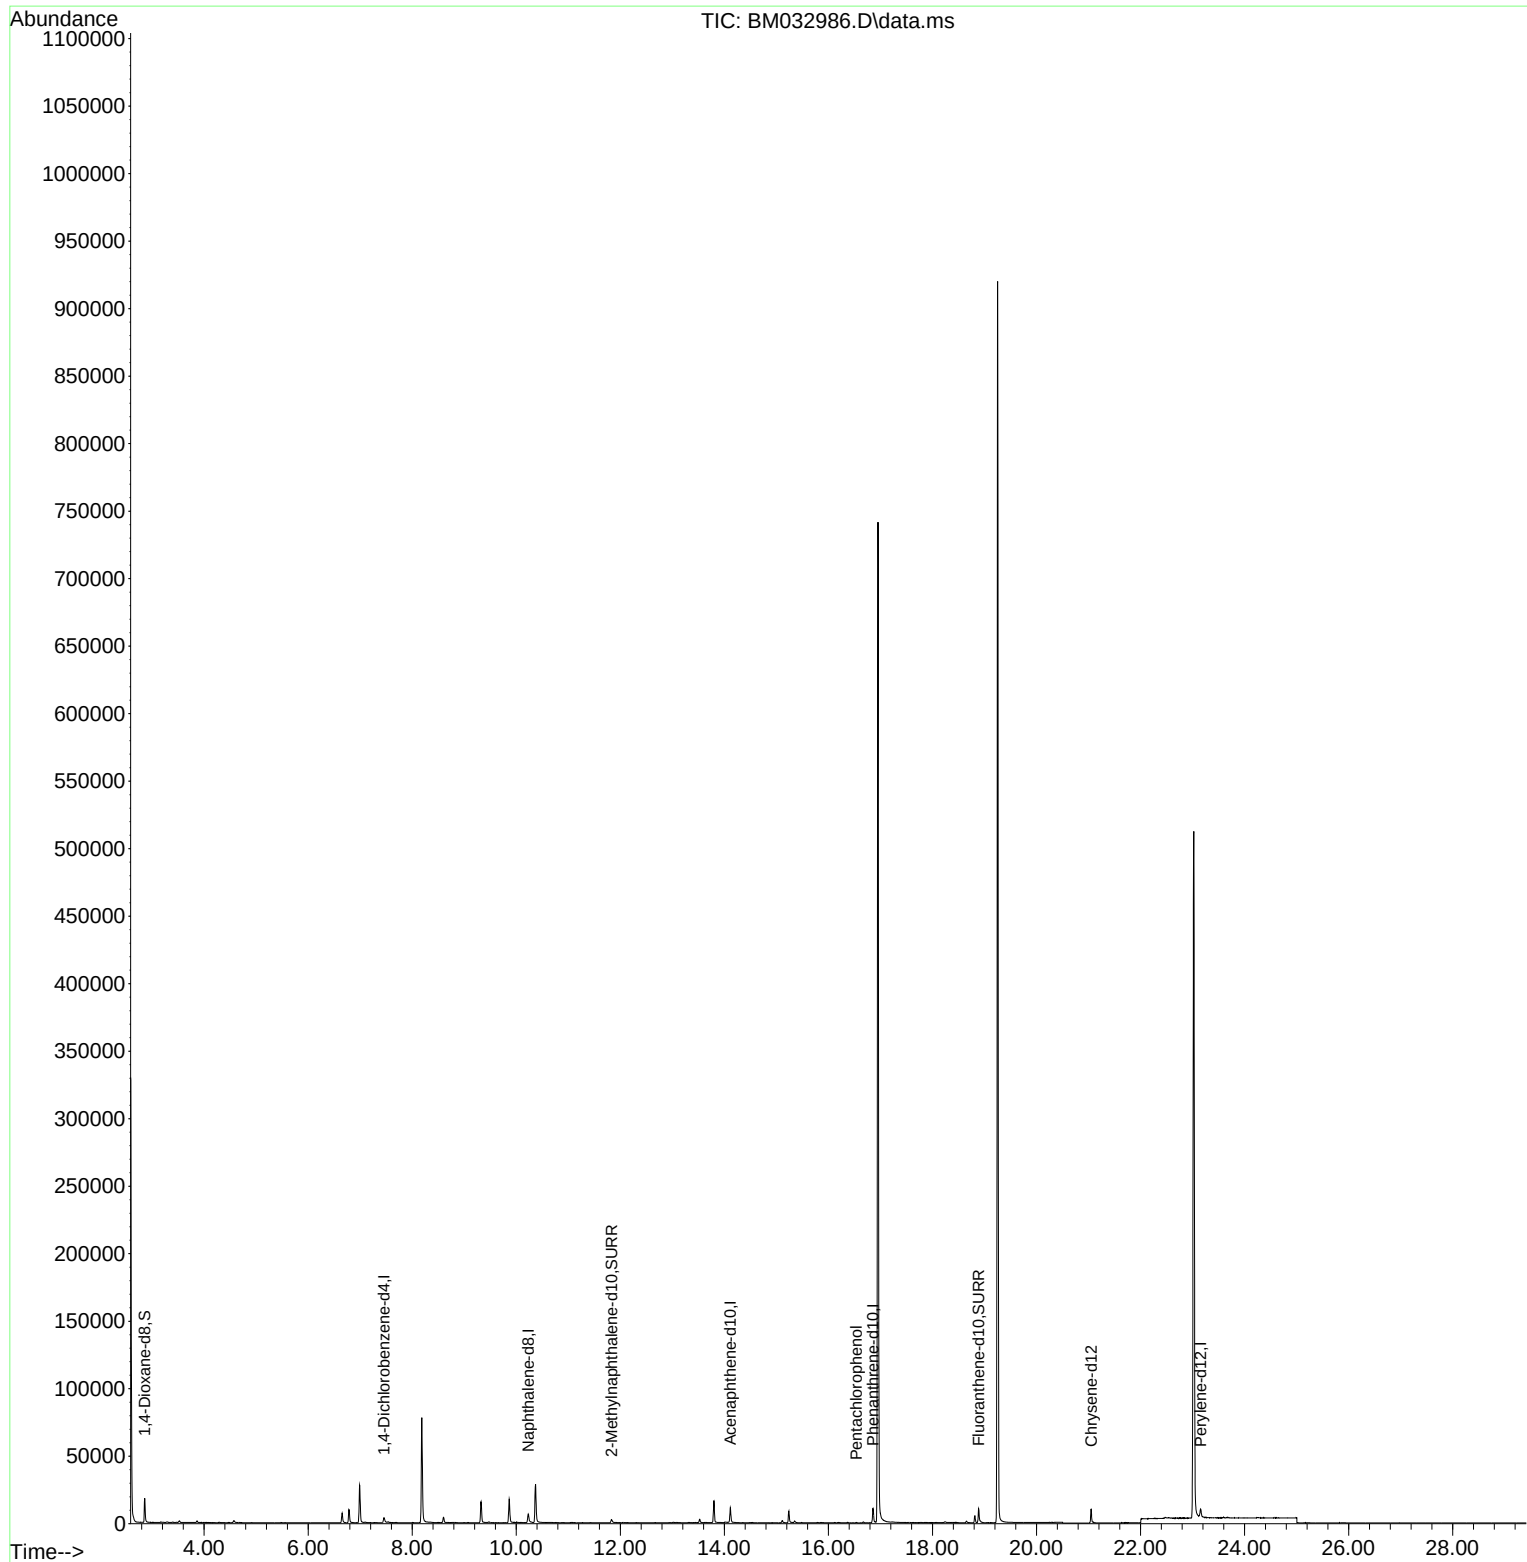

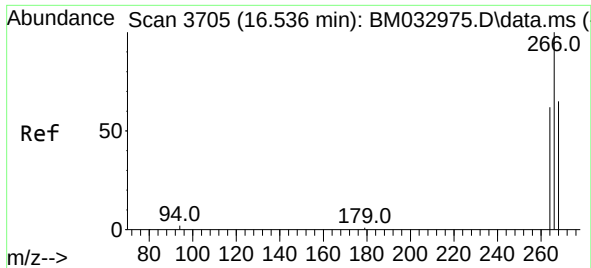

#14
 Pentachlorophenol
 Concen: 0.027 ng/ul
 RT: 16.539 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BM032986.D
 Acq: 11 Nov 2021 11:55

Instrument :
 BNA_M
 ClientSampleId :
 BG338

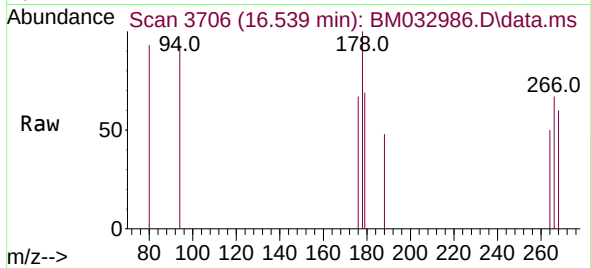

Tgt Ion:	266	Resp:	89
Ion Ratio	Lower	Upper	
266	100		
264	59.6	51.2	76.8
268	78.7	52.9	79.3

