

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM032992.D
 Acq On : 11 Nov 2021 16:35
 Operator : CG/JU
 Sample : M4615-02DL 5X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COV01DL

Quant Time: Nov 11 17:09:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 11 13:40:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.459	152	3011	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.230	136	9933	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.114	164	5661	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.858	188	10420	0.400	ng/ul	0.00
17) Chrysene-d12	21.062	240	6010	0.400	ng/ul	# 0.01
23) Perylene-d12	23.163	264	6274	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.864	96	1466	0.381	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.831	152	560	0.040	ng/ul	0.00
18) Fluoranthene-d10	18.892	212	905	0.050	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.280	128	191645	6.644	ng/ul	97
7) 2-Methylnaphthalene	11.903	142	10533	0.527	ng/ul	98
8) 1-Methylnaphthalene	12.128	142	5667	0.290	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM032992.D
Acq On : 11 Nov 2021 16:35
Operator : CG/JU
Sample : M4615-02DL 5X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0V01DL

Quant Time: Nov 11 17:09:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 11 13:40:18 2021
Response via : Initial Calibration




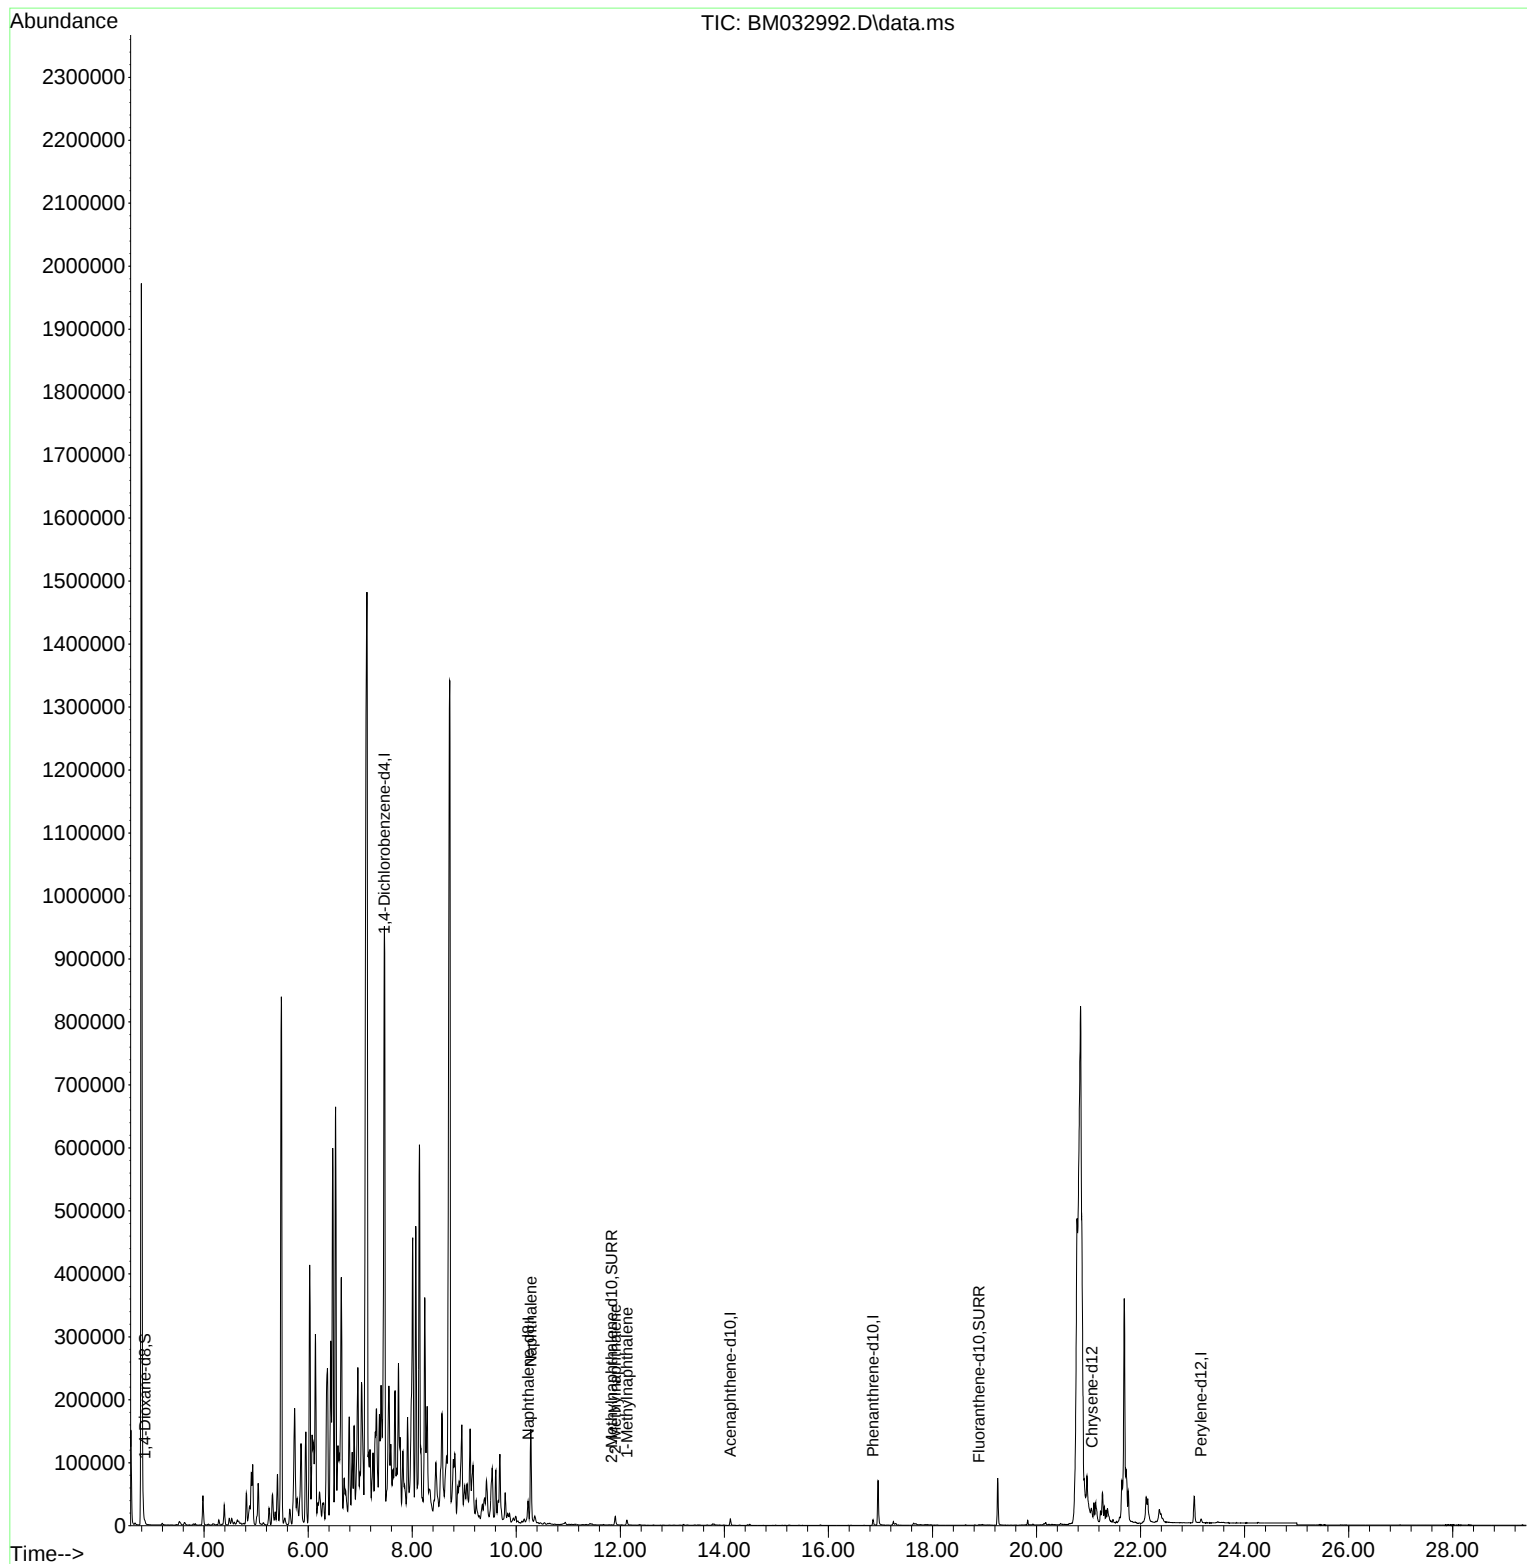


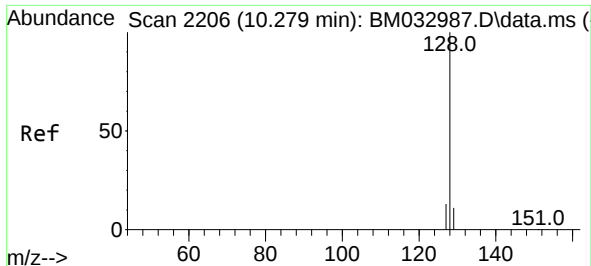

#5
Naphthalene
Concen: 6.644 ng/ul
RT: 10.280 min Scan# 21
Delta R.T. 0.001 min
Lab File: BM032992.D
Acq: 11 Nov 2021 16:35




Instrument :
BNA_M
ClientSampleId :
C0V01DL


Tgt Ion:128 Resp: 191645
Ion Ratio Lower Upper
128 100
129 11.2 9.8 14.6
127 13.2 11.8 17.8

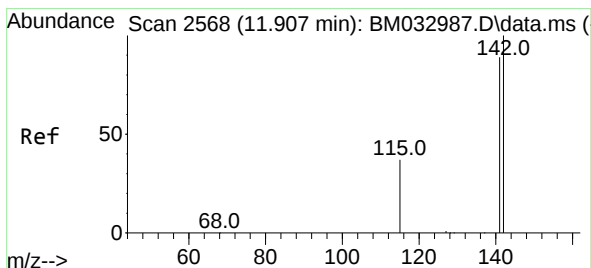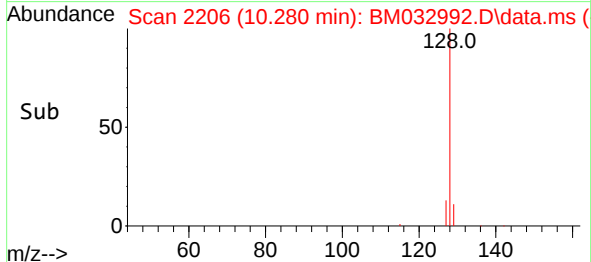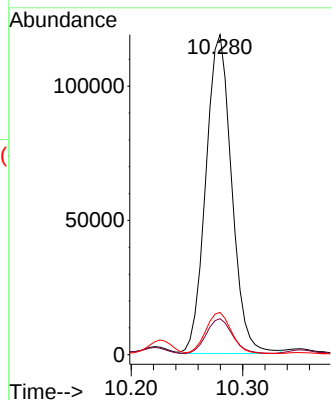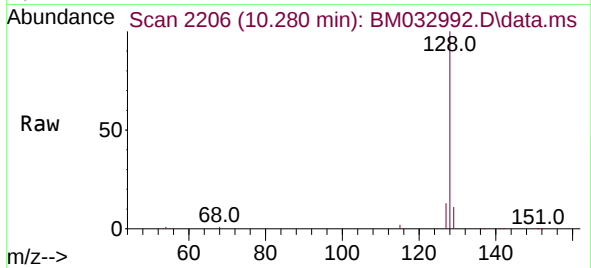

#7
2-Methylnaphthalene
Concen: 0.527 ng/ul
RT: 11.903 min Scan# 2567
Delta R.T. -0.003 min
Lab File: BM032992.D
Acq: 11 Nov 2021 16:35

Tgt Ion:142 Resp: 10533
Ion Ratio Lower Upper
142 100
141 90.1 73.3 109.9

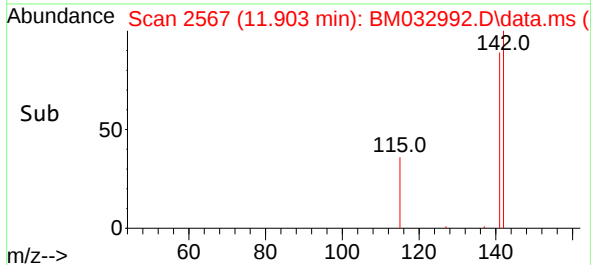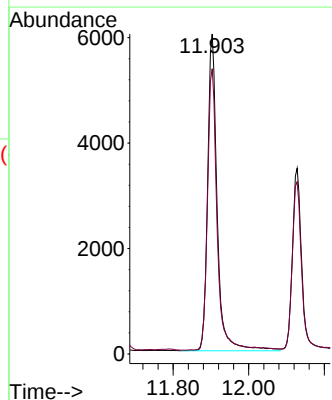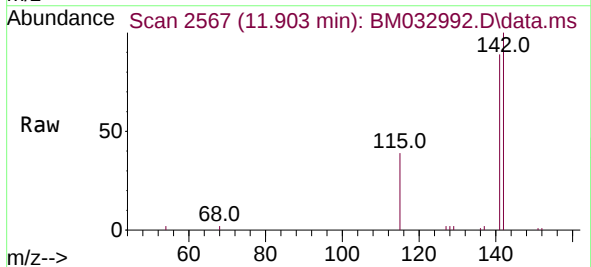

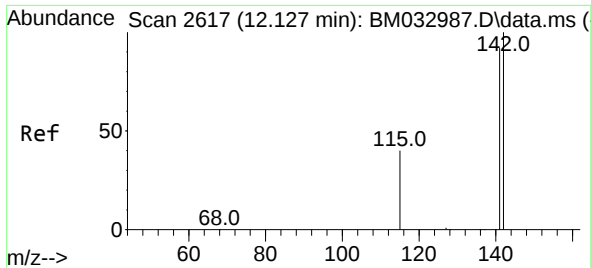

#8

1-Methylnaphthalene

Concen: 0.290 ng/ul

RT: 12.128 min Scan# 2

Delta R.T. 0.001 min

Lab File: BM032992.D


Acq: 11 Nov 2021 16:35

Instrument :

BNA_M

ClientSampleId :

C0V01DL

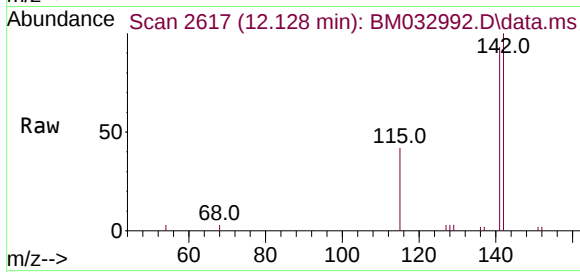

Tgt Ion:142 Resp: 5667

Ion Ratio Lower Upper

142 100

141 93.5 74.5 111.7

