

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
 Data File : BM033021.D
 Acq On : 12 Nov 2021 10:40
 Operator : CG/JU
 Sample : M4615-06
 Misc :
 ALS Vial : 117 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COV12

Quant Time: Nov 12 12:50:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 11 13:40:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.448	152	2411	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.225	136	8707	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.113	164	5423	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.855	188	11089	0.400	ng/ul	0.00
17) Chrysene-d12	21.047	240	8605	0.400	ng/ul	0.00
23) Perylene-d12	23.151	264	6703	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.864	96	11262	3.658	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.826	152	3496	0.283	ng/ul	0.00
18) Fluoranthene-d10	18.884	212	7583	0.291	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.274	128	2586	0.102	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110921\
Data File : BM033021.D
Acq On : 12 Nov 2021 10:40
Operator : CG/JU
Sample : M4615-06
Misc :
ALS Vial : 117 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0V12


Quant Time: Nov 12 12:50:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM110921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 11 13:40:18 2021
Response via : Initial Calibration

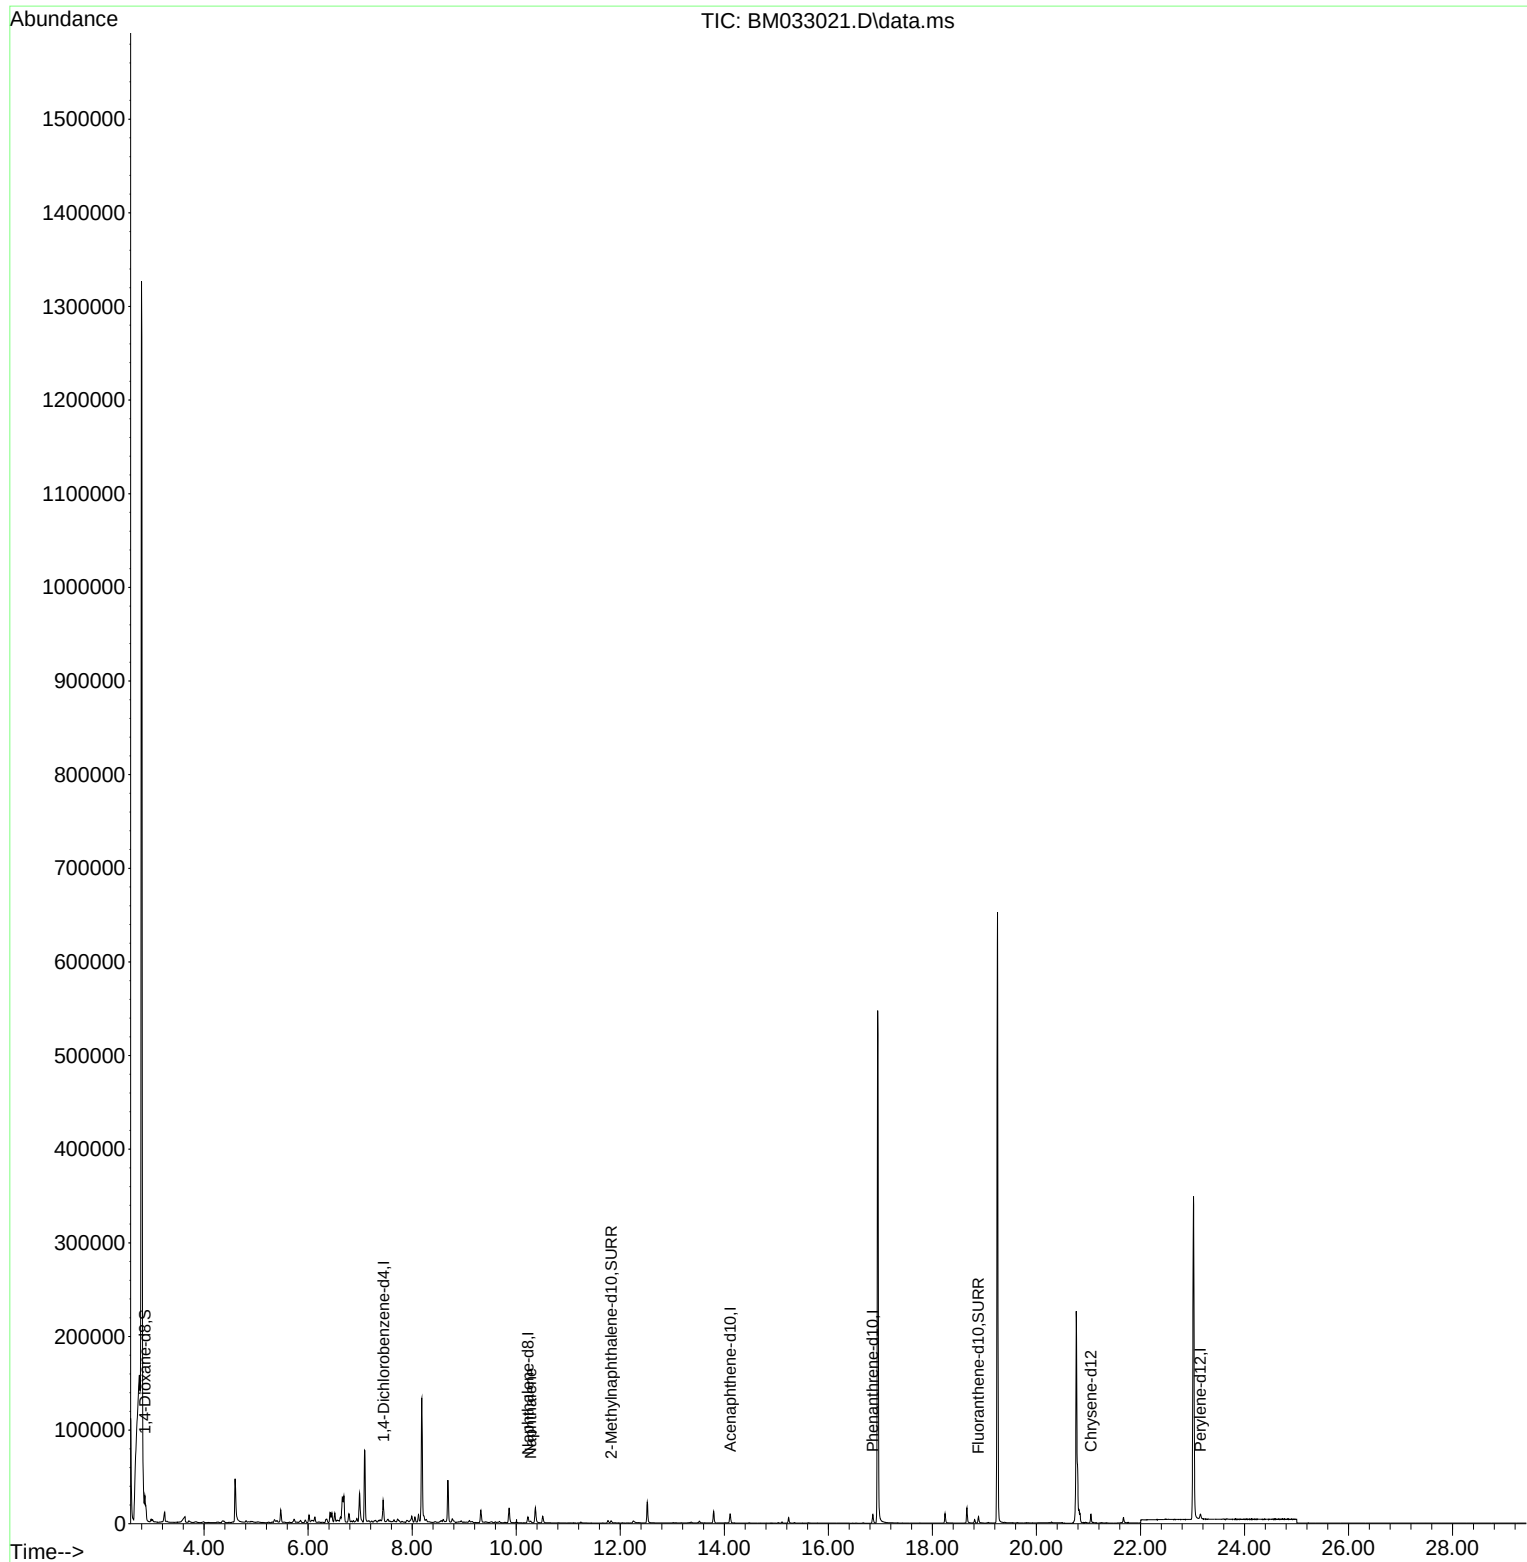

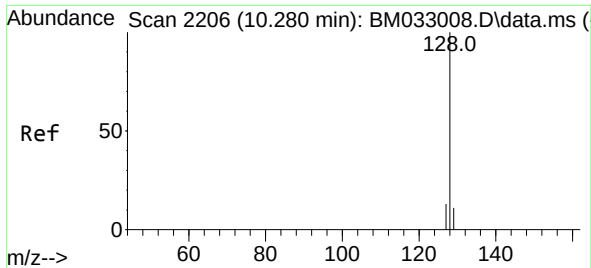

#5
Naphthalene
Concen: 0.102 ng/ul
RT: 10.274 min Scan# 21
Delta R.T. -0.005 min
Lab File: BM033021.D
Acq: 12 Nov 2021 10:40

Instrument :
BNA_M
ClientSampleId :
C0V12

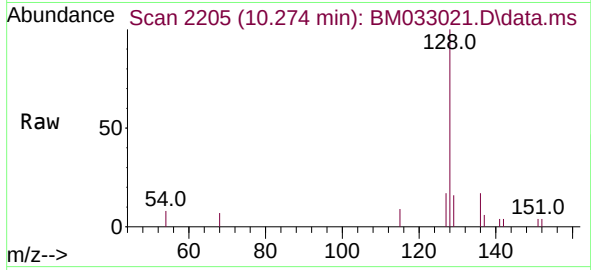

Tgt Ion:	128	Resp:	2586
Ion	Ratio	Lower	Upper
128	100		
129	15.9	9.8	14.6#
127	17.0	11.8	17.8

