


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM110921\  
 Data File : BM032906.D  
 Acq On : 09 Nov 2021 07:52  
 Operator : CG/JU  
 Sample : DFTPP025  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP025

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM110921.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Nov 09 13:31:56 2021

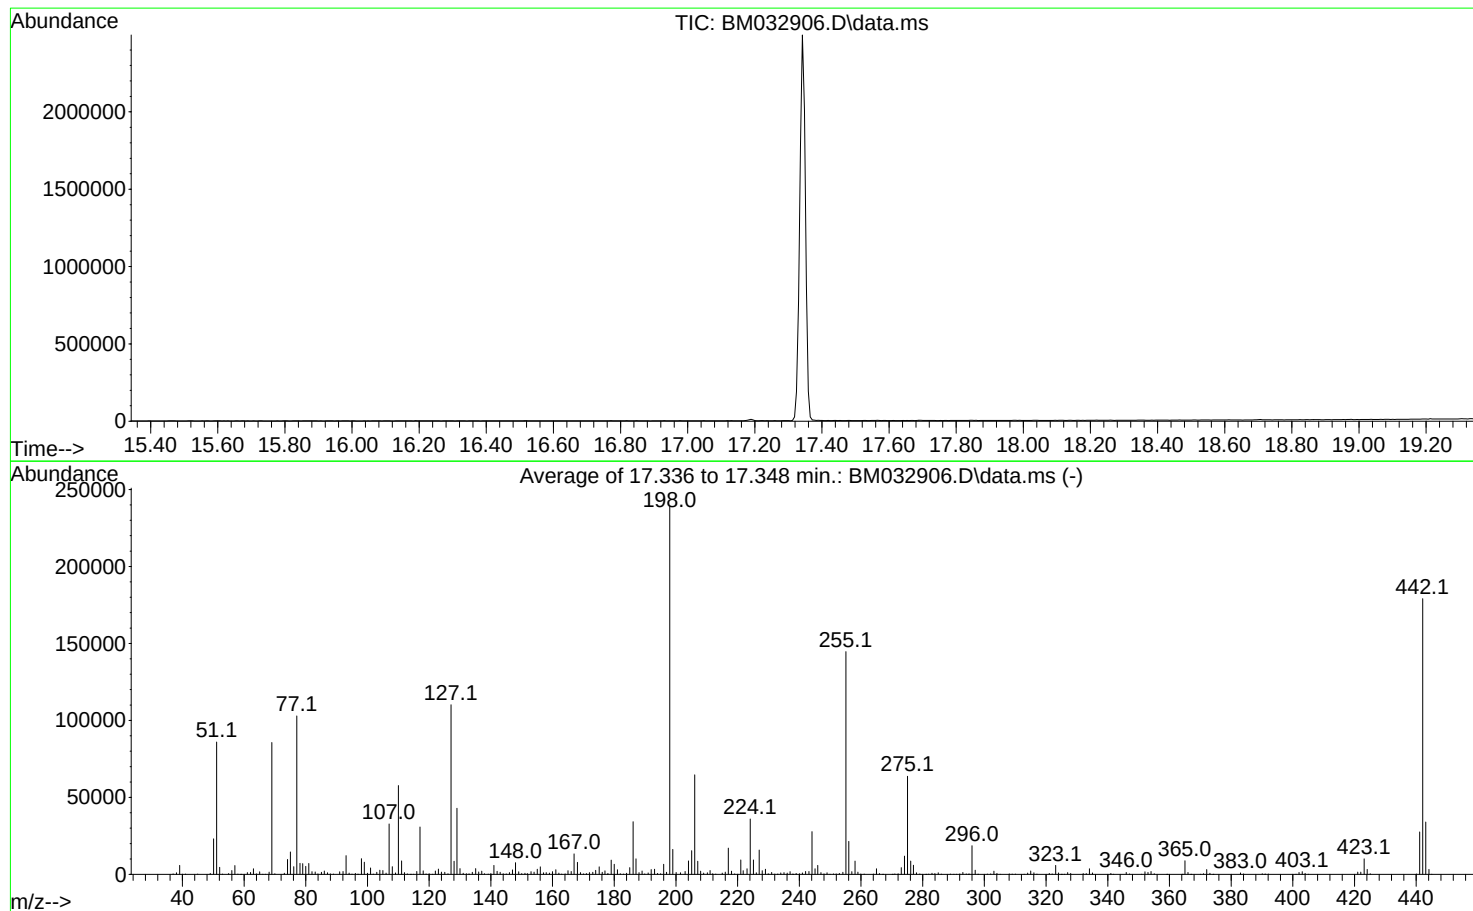

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.0         | 85947      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1511       | PASS                |
| 69             | 198             | 0.00            | 100             | 35.8         | 85635      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 454        | PASS                |
| 127            | 198             | 10              | 80              | 46.1         | 110147     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1399       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 238955     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 16204      | PASS                |
| 275            | 198             | 10              | 60              | 26.6         | 63669      | PASS                |
| 365            | 198             | 1               | 100             | 3.7          | 8803       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.5         | 27517      | PASS                |
| 442            | 198             | 50              | 100             | 74.9         | 179053     | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 33973      | PASS                |

| m/z    | Abundance |
|--------|-----------|
| 37.00  | 232.0     |
| 38.10  | 1041.0    |
| 39.10  | 5561.0    |
| 40.00  | 511.0     |
| 41.00  | 196.0     |
| 44.00  | 795.0     |
| 45.00  | 193.0     |
| 49.10  | 771.0     |
| 50.10  | 22128.0   |
| 51.10  | 85024.0   |
| 52.10  | 4736.0    |
| 53.00  | 191.0     |
| 55.00  | 504.0     |
| 56.00  | 2583.0    |
| 57.00  | 5297.0    |
| 58.00  | 263.0     |
| 58.90  | 165.0     |
| 61.10  | 1129.0    |
| 62.10  | 1199.0    |
| 63.00  | 3376.0    |
| 63.90  | 353.0     |
| 65.10  | 1710.0    |
| 67.00  | 170.0     |
| 68.10  | 1526.0    |
| 69.00  | 82856.0   |
| 70.00  | 414.0     |
| 73.10  | 1139.0    |
| 74.10  | 9407.0    |
| 75.00  | 14373.0   |
| 76.10  | 4732.0    |
| 77.10  | 99440.0   |
| 78.10  | 7391.0    |
| 79.00  | 6957.0    |
| 80.00  | 4762.0    |
| 81.00  | 6805.0    |
| 82.00  | 1755.0    |
| 83.00  | 1536.0    |
| 83.90  | 333.0     |
| 85.00  | 1350.0    |
| 86.00  | 2201.0    |
| 87.10  | 968.0     |
| 88.00  | 300.0     |
| 88.90  | 169.0     |
| 91.00  | 1659.0    |
| 92.10  | 1728.0    |
| 93.00  | 11497.0   |
| 94.10  | 824.0     |
| 95.00  | 203.0     |
| 96.10  | 603.0     |
| 96.80  | 184.0     |
| 97.20  | 209.0     |
| 98.10  | 9720.0    |
| 99.00  | 7917.0    |
| 100.00 | 739.0     |
| 101.00 | 3943.0    |
| 101.90 | 199.0     |
| 103.00 | 1328.0    |
| 104.00 | 2489.0    |
| 105.00 | 2565.0    |
| 106.10 | 970.0     |
| 107.00 | 31024.0   |
| 108.00 | 4570.0    |
| 109.10 | 818.0     |
| 110.00 | 52656.0   |
| 111.00 | 8572.0    |
| 112.00 | 1097.0    |
| 112.90 | 381.0     |
| 115.00 | 198.0     |
| 116.00 | 1692.0    |
| 117.00 | 28440.0   |
| 118.00 | 2204.0    |
| 118.90 | 290.0     |
| 120.00 | 486.0     |
| 122.00 | 2152.0    |
| 123.00 | 3218.0    |
| 124.00 | 1343.0    |
| 125.00 | 1170.0    |
| 126.10 | 627.0     |
| 127.10 | 100128.0  |
| 128.10 | 8057.0    |
| 129.00 | 39400.0   |
| 130.00 | 3665.0    |
| 131.00 | 703.0     |
| 132.00 | 332.0     |
| 132.90 | 224.0     |
| 134.00 | 1222.0    |
| 135.10 | 3096.0    |
| 136.10 | 1234.0    |
| 137.00 | 2087.0    |
| 137.90 | 336.0     |
| 140.00 | 444.0     |
| 141.00 | 5139.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 142.00 | 1706.0   |
| 143.00 | 1331.0   |
| 144.00 | 349.0    |
| 145.00 | 284.0    |
| 146.00 | 1100.0   |
| 147.00 | 2730.0   |
| 148.00 | 6677.0   |
| 149.00 | 1629.0   |
| 150.00 | 462.0    |
| 151.00 | 726.0    |
| 151.80 | 428.0    |
| 153.00 | 1641.0   |
| 154.00 | 1388.0   |
| 155.00 | 2809.0   |
| 156.00 | 4539.0   |
| 157.00 | 925.0    |
| 158.00 | 964.0    |
| 159.00 | 883.0    |
| 160.00 | 1501.0   |
| 161.00 | 2295.0   |
| 162.10 | 700.0    |
| 162.90 | 193.0    |
| 164.10 | 252.0    |
| 165.00 | 1994.0   |
| 166.10 | 1668.0   |
| 167.00 | 11736.0  |
| 168.00 | 7142.0   |
| 169.00 | 1181.0   |
| 170.10 | 253.0    |
| 171.00 | 452.0    |
| 172.00 | 832.0    |
| 173.00 | 1164.0   |
| 174.00 | 2371.0   |
| 175.10 | 4069.0   |
| 176.10 | 1182.0   |
| 177.00 | 1967.0   |
| 177.80 | 622.0    |
| 179.00 | 7951.0   |
| 180.00 | 5819.0   |
| 181.00 | 2860.0   |
| 182.00 | 368.0    |
| 183.00 | 267.0    |
| 184.00 | 627.0    |
| 185.10 | 3935.0   |
| 186.10 | 28520.0  |
| 187.00 | 9052.0   |
| 188.00 | 1162.0   |
| 189.00 | 1851.0   |
| 189.90 | 319.0    |
| 191.10 | 965.0    |
| 192.00 | 2772.0   |
| 193.00 | 3130.0   |
| 194.00 | 618.0    |
| 195.00 | 405.0    |
| 196.10 | 5414.0   |
| 197.00 | 1056.0   |
| 198.00 | 204672.0 |
| 199.00 | 14187.0  |
| 200.10 | 1201.0   |
| 201.60 | 897.0    |
| 203.00 | 1583.0   |
| 204.00 | 7329.0   |
| 205.10 | 12785.0  |
| 206.10 | 53936.0  |
| 207.10 | 8480.0   |
| 208.00 | 1830.0   |
| 209.00 | 964.0    |
| 210.20 | 979.0    |
| 211.00 | 2175.0   |
| 211.80 | 624.0    |
| 212.90 | 186.0    |
| 215.00 | 636.0    |
| 216.00 | 1144.0   |
| 217.00 | 14124.0  |
| 218.00 | 1735.0   |
| 219.00 | 248.0    |
| 221.10 | 7838.0   |
| 221.70 | 2041.0   |
| 223.10 | 2864.0   |
| 224.10 | 29584.0  |
| 225.10 | 7705.0   |
| 226.00 | 891.0    |
| 227.00 | 12405.0  |
| 228.00 | 1999.0   |
| 229.00 | 2727.0   |
| 229.90 | 352.0    |
| 231.10 | 887.0    |
| 232.00 | 169.0    |
| 232.90 | 211.0    |
| 234.00 | 854.0    |
| 235.10 | 940.0    |
| 236.10 | 587.0    |
| 237.00 | 1670.0   |
| 237.90 | 332.0    |
| 239.00 | 622.0    |
| 240.10 | 374.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 241.00 | 668.0    |
| 242.00 | 1534.0   |
| 243.10 | 1591.0   |
| 244.10 | 21704.0  |
| 245.10 | 2985.0   |
| 246.00 | 4520.0   |
| 247.00 | 1030.0   |
| 248.00 | 245.0    |
| 249.00 | 863.0    |
| 251.00 | 255.0    |
| 252.00 | 292.0    |
| 253.00 | 511.0    |
| 254.10 | 1172.0   |
| 255.10 | 114176.0 |
| 256.00 | 17872.0  |
| 257.00 | 1432.0   |
| 258.00 | 6612.0   |
| 259.00 | 1166.0   |
| 260.00 | 222.0    |
| 261.00 | 186.0    |
| 265.00 | 3004.0   |
| 266.00 | 486.0    |
| 271.00 | 296.0    |
| 271.90 | 292.0    |
| 273.00 | 3309.0   |
| 274.10 | 9127.0   |
| 275.10 | 49744.0  |
| 276.10 | 6937.0   |
| 277.00 | 4721.0   |
| 278.00 | 810.0    |
| 279.00 | 277.0    |
| 281.10 | 205.0    |
| 283.00 | 589.0    |
| 284.00 | 340.0    |
| 285.10 | 754.0    |
| 286.00 | 162.0    |
| 289.00 | 206.0    |
| 292.00 | 216.0    |
| 293.00 | 925.0    |
| 294.10 | 369.0    |
| 294.90 | 349.0    |
| 296.00 | 14155.0  |
| 297.00 | 2111.0   |
| 297.90 | 206.0    |
| 300.90 | 185.0    |
| 302.00 | 266.0    |
| 303.10 | 1520.0   |
| 304.00 | 366.0    |
| 308.00 | 288.0    |
| 309.10 | 162.0    |
| 310.10 | 164.0    |
| 314.00 | 656.0    |
| 315.00 | 1642.0   |
| 316.00 | 866.0    |
| 321.00 | 429.0    |
| 322.00 | 243.0    |
| 323.10 | 4255.0   |
| 324.00 | 733.0    |
| 326.00 | 150.0    |
| 327.00 | 972.0    |
| 328.00 | 528.0    |
| 332.00 | 362.0    |
| 332.90 | 362.0    |
| 334.00 | 2705.0   |
| 335.10 | 720.0    |
| 341.00 | 419.0    |
| 346.00 | 882.0    |
| 347.10 | 253.0    |
| 352.00 | 1353.0   |
| 353.10 | 817.0    |
| 354.00 | 1517.0   |
| 355.10 | 323.0    |
| 365.00 | 5973.0   |
| 366.00 | 924.0    |
| 371.00 | 278.0    |
| 372.00 | 2164.0   |
| 373.10 | 496.0    |
| 383.00 | 559.0    |
| 384.10 | 207.0    |
| 390.00 | 323.0    |
| 390.90 | 210.0    |
| 392.10 | 175.0    |
| 402.00 | 944.0    |
| 403.10 | 1395.0   |
| 404.00 | 494.0    |
| 421.00 | 1012.0   |
| 422.10 | 943.0    |
| 423.10 | 6774.0   |
| 424.10 | 2806.0   |
| 425.10 | 490.0    |
| 441.10 | 17968.0  |
| 442.10 | 115528.0 |
| 443.10 | 22576.0  |
| 444.10 | 2054.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

| m/z    | Abundance |
|--------|-----------|
| 40.00  | 435.0     |
| 44.00  | 866.0     |
| 49.00  | 173.0     |
| 73.10  | 525.0     |
| 147.00 | 172.0     |
| 190.90 | 161.0     |
| 193.10 | 183.0     |
| 207.00 | 913.0     |
| 208.10 | 255.0     |
| 208.90 | 182.0     |
| 281.00 | 249.0     |

**Instrument :**  
BNA\_M  
**ClientSampleId :**  
DFTPP025

| m/z    | Abundance |
|--------|-----------|
| 37.00  | 386.0     |
| 38.10  | 1298.0    |
| 39.10  | 7034.0    |
| 40.10  | 544.0     |
| 41.00  | 202.0     |
| 44.00  | 763.0     |
| 45.00  | 227.0     |
| 49.00  | 1015.0    |
| 50.10  | 28208.0   |
| 51.10  | 103032.0  |
| 52.10  | 5530.0    |
| 52.90  | 190.0     |
| 55.00  | 521.0     |
| 56.00  | 2896.0    |
| 57.00  | 6934.0    |
| 58.00  | 278.0     |
| 61.00  | 1250.0    |
| 62.10  | 1467.0    |
| 63.10  | 4568.0    |
| 64.10  | 652.0     |
| 65.10  | 1895.0    |
| 66.10  | 181.0     |
| 67.00  | 185.0     |
| 68.10  | 1715.0    |
| 69.00  | 103056.0  |
| 70.00  | 599.0     |
| 73.10  | 1338.0    |
| 74.10  | 11569.0   |
| 75.00  | 17128.0   |
| 76.10  | 5976.0    |
| 77.10  | 122592.0  |
| 78.10  | 8515.0    |
| 79.00  | 8110.0    |
| 80.00  | 6373.0    |
| 81.00  | 8260.0    |
| 82.00  | 2009.0    |
| 83.00  | 1782.0    |
| 84.00  | 385.0     |
| 85.10  | 1631.0    |
| 86.00  | 2486.0    |
| 87.10  | 1312.0    |
| 88.00  | 466.0     |
| 88.90  | 181.0     |
| 91.00  | 1902.0    |
| 92.00  | 2277.0    |
| 93.10  | 14459.0   |
| 94.00  | 957.0     |
| 95.00  | 248.0     |
| 96.10  | 683.0     |
| 96.90  | 262.0     |
| 98.00  | 11863.0   |
| 99.00  | 9634.0    |
| 100.00 | 912.0     |
| 101.00 | 5094.0    |
| 101.90 | 272.0     |
| 103.00 | 1472.0    |
| 104.00 | 3110.0    |
| 105.00 | 2895.0    |
| 106.00 | 794.0     |
| 107.00 | 38968.0   |
| 108.00 | 5781.0    |
| 109.10 | 1146.0    |
| 110.00 | 69464.0   |
| 111.00 | 10549.0   |
| 112.00 | 1353.0    |
| 113.00 | 393.0     |
| 113.90 | 154.0     |
| 115.00 | 165.0     |
| 116.00 | 2243.0    |
| 117.00 | 36896.0   |
| 118.10 | 2794.0    |
| 119.00 | 373.0     |
| 120.00 | 475.0     |
| 121.20 | 265.0     |
| 122.00 | 2667.0    |
| 123.00 | 4053.0    |
| 124.00 | 1862.0    |
| 125.00 | 1710.0    |
| 127.10 | 133632.0  |
| 128.00 | 9980.0    |
| 129.00 | 51880.0   |
| 130.00 | 4710.0    |
| 131.10 | 921.0     |
| 132.00 | 529.0     |
| 132.90 | 354.0     |
| 134.00 | 1627.0    |
| 135.10 | 4499.0    |
| 136.00 | 1749.0    |
| 137.10 | 2524.0    |
| 138.00 | 555.0     |
| 139.10 | 423.0     |
| 140.00 | 672.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 141.00 | 7532.0   |
| 142.10 | 2555.0   |
| 143.00 | 1653.0   |
| 144.00 | 500.0    |
| 145.00 | 265.0    |
| 146.10 | 1217.0   |
| 147.00 | 3799.0   |
| 148.00 | 9148.0   |
| 149.00 | 1986.0   |
| 150.00 | 566.0    |
| 151.10 | 854.0    |
| 151.90 | 708.0    |
| 153.00 | 2070.0   |
| 154.00 | 1853.0   |
| 155.10 | 4147.0   |
| 156.10 | 5844.0   |
| 157.10 | 1302.0   |
| 157.90 | 1423.0   |
| 159.00 | 1034.0   |
| 160.00 | 2231.0   |
| 161.10 | 4051.0   |
| 162.00 | 1019.0   |
| 163.00 | 307.0    |
| 164.10 | 423.0    |
| 165.00 | 2984.0   |
| 166.10 | 2151.0   |
| 167.00 | 15789.0  |
| 168.00 | 9236.0   |
| 169.10 | 1223.0   |
| 170.00 | 518.0    |
| 170.90 | 567.0    |
| 172.00 | 1502.0   |
| 173.00 | 1668.0   |
| 174.00 | 3217.0   |
| 175.10 | 6092.0   |
| 176.10 | 1632.0   |
| 177.00 | 2718.0   |
| 178.00 | 874.0    |
| 179.00 | 10696.0  |
| 180.00 | 7771.0   |
| 181.00 | 3619.0   |
| 182.00 | 518.0    |
| 183.00 | 273.0    |
| 184.00 | 922.0    |
| 185.00 | 5035.0   |
| 186.10 | 41616.0  |
| 187.10 | 11874.0  |
| 188.10 | 1374.0   |
| 189.00 | 2512.0   |
| 189.90 | 408.0    |
| 191.00 | 1352.0   |
| 192.00 | 3769.0   |
| 193.10 | 3986.0   |
| 194.10 | 732.0    |
| 195.10 | 568.0    |
| 196.10 | 8082.0   |
| 197.00 | 1811.0   |
| 198.00 | 282752.0 |
| 199.00 | 19176.0  |
| 200.00 | 1505.0   |
| 201.40 | 1372.0   |
| 203.00 | 2094.0   |
| 204.10 | 10392.0  |
| 205.10 | 17784.0  |
| 206.10 | 77400.0  |
| 207.10 | 11114.0  |
| 208.00 | 2925.0   |
| 209.00 | 1114.0   |
| 210.20 | 1222.0   |
| 211.10 | 2913.0   |
| 212.00 | 442.0    |
| 213.00 | 239.0    |
| 215.00 | 1038.0   |
| 216.00 | 1825.0   |
| 217.00 | 20448.0  |
| 218.00 | 2555.0   |
| 219.10 | 255.0    |
| 221.00 | 10865.0  |
| 221.80 | 2839.0   |
| 223.00 | 4382.0   |
| 224.10 | 43280.0  |
| 225.10 | 11660.0  |
| 226.10 | 1303.0   |
| 227.00 | 19664.0  |
| 228.00 | 2928.0   |
| 229.00 | 3868.0   |
| 229.90 | 536.0    |
| 231.00 | 1451.0   |
| 232.10 | 347.0    |
| 233.10 | 304.0    |
| 234.00 | 1153.0   |
| 235.10 | 1232.0   |
| 236.00 | 1084.0   |
| 237.00 | 2013.0   |
| 238.10 | 337.0    |
| 239.00 | 679.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 240.00 | 505.0    |
| 241.00 | 1092.0   |
| 242.00 | 2146.0   |
| 243.10 | 2199.0   |
| 244.10 | 34080.0  |
| 245.10 | 4379.0   |
| 246.00 | 7010.0   |
| 247.00 | 1371.0   |
| 248.00 | 361.0    |
| 249.00 | 1103.0   |
| 249.90 | 290.0    |
| 251.00 | 325.0    |
| 252.00 | 297.0    |
| 253.00 | 753.0    |
| 254.10 | 1672.0   |
| 255.10 | 172096.0 |
| 256.10 | 25432.0  |
| 257.10 | 2296.0   |
| 258.10 | 10269.0  |
| 259.00 | 1752.0   |
| 259.90 | 265.0    |
| 261.10 | 287.0    |
| 264.00 | 354.0    |
| 265.00 | 4336.0   |
| 266.00 | 560.0    |
| 270.10 | 166.0    |
| 271.00 | 481.0    |
| 272.10 | 521.0    |
| 273.10 | 5378.0   |
| 274.10 | 14266.0  |
| 275.10 | 75968.0  |
| 276.10 | 9956.0   |
| 277.00 | 7069.0   |
| 278.00 | 1217.0   |
| 279.00 | 235.0    |
| 281.00 | 323.0    |
| 281.90 | 298.0    |
| 283.00 | 810.0    |
| 284.00 | 659.0    |
| 285.10 | 1200.0   |
| 286.00 | 257.0    |
| 289.00 | 306.0    |
| 290.10 | 225.0    |
| 291.00 | 183.0    |
| 292.00 | 310.0    |
| 293.00 | 1509.0   |
| 294.10 | 410.0    |
| 295.10 | 454.0    |
| 296.00 | 21576.0  |
| 297.00 | 3418.0   |
| 298.10 | 195.0    |
| 301.00 | 276.0    |
| 302.10 | 421.0    |
| 303.10 | 2732.0   |
| 304.10 | 795.0    |
| 305.10 | 202.0    |
| 308.10 | 261.0    |
| 308.90 | 203.0    |
| 310.00 | 258.0    |
| 312.90 | 162.0    |
| 314.00 | 868.0    |
| 315.00 | 2444.0   |
| 316.10 | 1262.0   |
| 317.00 | 255.0    |
| 321.10 | 808.0    |
| 322.00 | 296.0    |
| 323.10 | 6787.0   |
| 324.10 | 1033.0   |
| 324.90 | 154.0    |
| 325.90 | 194.0    |
| 327.00 | 1240.0   |
| 328.00 | 763.0    |
| 332.00 | 589.0    |
| 333.00 | 561.0    |
| 334.00 | 4187.0   |
| 335.00 | 1107.0   |
| 341.00 | 816.0    |
| 342.00 | 248.0    |
| 346.00 | 1656.0   |
| 347.00 | 412.0    |
| 351.00 | 170.0    |
| 352.00 | 1878.0   |
| 353.00 | 1686.0   |
| 354.10 | 2159.0   |
| 355.10 | 504.0    |
| 364.10 | 158.0    |
| 365.00 | 10697.0  |
| 366.00 | 1386.0   |
| 366.90 | 159.0    |
| 370.10 | 222.0    |
| 371.10 | 426.0    |
| 372.10 | 3619.0   |
| 373.10 | 955.0    |
| 374.10 | 162.0    |
| 383.00 | 1072.0   |
| 384.00 | 346.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025



|        |          |
|--------|----------|
| 390.10 | 450.0    |
| 391.10 | 299.0    |
| 392.00 | 209.0    |
| 401.00 | 184.0    |
| 402.00 | 1461.0   |
| 403.00 | 2008.0   |
| 404.00 | 673.0    |
| 405.00 | 243.0    |
| 421.00 | 1459.0   |
| 422.00 | 1637.0   |
| 423.10 | 11614.0  |
| 424.10 | 3502.0   |
| 425.10 | 429.0    |
| 440.10 | 286.0    |
| 441.10 | 32336.0  |
| 442.10 | 208384.0 |
| 443.10 | 39008.0  |
| 444.10 | 3990.0   |
| 445.00 | 237.0    |

|                  |
|------------------|
| Instrument :     |
| BNA_M            |
| ClientSampleId : |
| DFTPP025         |

| m/z    | Abundance |
|--------|-----------|
| 37.00  | 324.0     |
| 38.10  | 794.0     |
| 39.10  | 4967.0    |
| 40.00  | 507.0     |
| 41.10  | 239.0     |
| 44.00  | 899.0     |
| 45.00  | 185.0     |
| 49.00  | 653.0     |
| 50.10  | 18784.0   |
| 51.10  | 69784.0   |
| 52.10  | 3440.0    |
| 53.00  | 169.0     |
| 55.00  | 404.0     |
| 56.00  | 1881.0    |
| 57.00  | 4801.0    |
| 58.00  | 201.0     |
| 61.00  | 964.0     |
| 62.10  | 1214.0    |
| 63.10  | 2976.0    |
| 64.00  | 416.0     |
| 65.00  | 1399.0    |
| 68.10  | 1293.0    |
| 69.00  | 70992.0   |
| 70.00  | 348.0     |
| 73.00  | 1378.0    |
| 74.10  | 7948.0    |
| 75.00  | 12252.0   |
| 76.10  | 4272.0    |
| 77.10  | 86680.0   |
| 78.10  | 5646.0    |
| 79.00  | 5759.0    |
| 80.00  | 4466.0    |
| 81.00  | 6267.0    |
| 82.00  | 1478.0    |
| 83.10  | 1406.0    |
| 83.90  | 348.0     |
| 85.00  | 1091.0    |
| 86.00  | 1860.0    |
| 87.00  | 806.0     |
| 88.00  | 288.0     |
| 89.00  | 166.0     |
| 91.00  | 1446.0    |
| 92.00  | 1537.0    |
| 93.00  | 10508.0   |
| 94.00  | 715.0     |
| 95.00  | 218.0     |
| 96.00  | 505.0     |
| 97.10  | 193.0     |
| 98.00  | 8937.0    |
| 99.00  | 6193.0    |
| 100.00 | 666.0     |
| 101.00 | 3466.0    |
| 102.00 | 156.0     |
| 103.00 | 1191.0    |
| 104.00 | 2374.0    |
| 105.00 | 2051.0    |
| 106.00 | 699.0     |
| 107.00 | 28296.0   |
| 108.10 | 4531.0    |
| 109.10 | 830.0     |
| 110.00 | 51056.0   |
| 111.10 | 7056.0    |
| 112.00 | 962.0     |
| 113.00 | 316.0     |
| 116.00 | 1621.0    |
| 117.00 | 27096.0   |
| 118.00 | 1982.0    |
| 119.10 | 228.0     |
| 120.10 | 315.0     |
| 121.00 | 169.0     |
| 122.00 | 1812.0    |
| 123.00 | 3066.0    |
| 124.00 | 1217.0    |
| 125.10 | 1233.0    |
| 126.10 | 555.0     |
| 127.10 | 96680.0   |
| 128.00 | 7452.0    |
| 129.00 | 37440.0   |
| 130.00 | 2855.0    |
| 131.00 | 644.0     |
| 132.10 | 391.0     |
| 132.90 | 219.0     |
| 133.10 | 213.0     |
| 134.00 | 1337.0    |
| 135.10 | 3561.0    |
| 136.00 | 1559.0    |
| 137.10 | 1624.0    |
| 138.00 | 402.0     |
| 139.10 | 197.0     |
| 140.00 | 513.0     |
| 141.00 | 4922.0    |
| 142.00 | 1796.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 143.00 | 1122.0   |
| 144.00 | 420.0    |
| 145.00 | 253.0    |
| 145.90 | 1082.0   |
| 147.00 | 2860.0   |
| 148.00 | 6973.0   |
| 149.10 | 1480.0   |
| 150.00 | 416.0    |
| 151.00 | 706.0    |
| 151.90 | 406.0    |
| 153.00 | 1749.0   |
| 154.00 | 1233.0   |
| 155.00 | 3089.0   |
| 156.10 | 4412.0   |
| 157.10 | 862.0    |
| 158.00 | 935.0    |
| 159.00 | 637.0    |
| 159.90 | 1689.0   |
| 161.00 | 2608.0   |
| 162.00 | 750.0    |
| 163.10 | 267.0    |
| 164.00 | 234.0    |
| 165.00 | 2117.0   |
| 166.00 | 1741.0   |
| 167.00 | 12536.0  |
| 168.10 | 6911.0   |
| 169.00 | 1141.0   |
| 170.00 | 316.0    |
| 171.00 | 431.0    |
| 171.90 | 1088.0   |
| 173.10 | 1092.0   |
| 174.00 | 2362.0   |
| 175.10 | 4449.0   |
| 176.10 | 1220.0   |
| 177.00 | 2161.0   |
| 177.90 | 732.0    |
| 179.00 | 9056.0   |
| 180.00 | 6092.0   |
| 181.10 | 2484.0   |
| 181.90 | 433.0    |
| 183.00 | 241.0    |
| 184.00 | 664.0    |
| 185.10 | 4001.0   |
| 186.10 | 32376.0  |
| 187.00 | 9329.0   |
| 188.00 | 1052.0   |
| 189.00 | 2076.0   |
| 189.90 | 371.0    |
| 191.00 | 1019.0   |
| 192.00 | 2745.0   |
| 193.10 | 3303.0   |
| 194.00 | 658.0    |
| 195.00 | 360.0    |
| 196.00 | 6233.0   |
| 196.80 | 1330.0   |
| 198.00 | 229440.0 |
| 199.00 | 15248.0  |
| 200.00 | 1068.0   |
| 201.40 | 990.0    |
| 203.00 | 1856.0   |
| 204.10 | 8357.0   |
| 205.10 | 15522.0  |
| 206.10 | 62648.0  |
| 207.10 | 8674.0   |
| 208.00 | 2362.0   |
| 209.10 | 896.0    |
| 210.20 | 1045.0   |
| 211.10 | 2385.0   |
| 211.90 | 405.0    |
| 213.00 | 233.0    |
| 215.00 | 765.0    |
| 216.00 | 1287.0   |
| 217.00 | 16480.0  |
| 218.00 | 2104.0   |
| 219.00 | 288.0    |
| 220.10 | 377.0    |
| 221.10 | 9398.0   |
| 221.90 | 2316.0   |
| 223.00 | 3550.0   |
| 224.10 | 35088.0  |
| 225.10 | 8623.0   |
| 226.10 | 1072.0   |
| 227.00 | 15202.0  |
| 228.00 | 2268.0   |
| 229.00 | 3308.0   |
| 230.10 | 485.0    |
| 231.00 | 1450.0   |
| 232.10 | 267.0    |
| 233.00 | 244.0    |
| 234.00 | 951.0    |
| 235.00 | 1130.0   |
| 236.10 | 862.0    |
| 237.00 | 1522.0   |
| 237.90 | 221.0    |
| 238.90 | 626.0    |
| 240.00 | 415.0    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 241.00 | 1115.0   |
| 242.10 | 2055.0   |
| 243.10 | 1877.0   |
| 244.10 | 27568.0  |
| 245.10 | 3573.0   |
| 246.00 | 5850.0   |
| 247.00 | 1015.0   |
| 248.00 | 262.0    |
| 249.00 | 1064.0   |
| 250.00 | 170.0    |
| 251.10 | 322.0    |
| 251.90 | 276.0    |
| 253.00 | 727.0    |
| 254.10 | 1325.0   |
| 255.10 | 147776.0 |
| 256.10 | 20848.0  |
| 257.00 | 1484.0   |
| 258.00 | 8988.0   |
| 259.00 | 1531.0   |
| 259.90 | 230.0    |
| 260.90 | 249.0    |
| 264.10 | 211.0    |
| 265.00 | 3724.0   |
| 266.00 | 492.0    |
| 267.00 | 150.0    |
| 271.00 | 295.0    |
| 272.00 | 425.0    |
| 273.00 | 4466.0   |
| 274.10 | 12235.0  |
| 275.10 | 65296.0  |
| 276.10 | 8895.0   |
| 277.00 | 6019.0   |
| 278.00 | 1018.0   |
| 279.10 | 360.0    |
| 281.00 | 268.0    |
| 282.00 | 244.0    |
| 283.00 | 661.0    |
| 283.90 | 524.0    |
| 285.00 | 1181.0   |
| 286.00 | 254.0    |
| 289.00 | 215.0    |
| 292.10 | 315.0    |
| 293.10 | 1446.0   |
| 294.10 | 313.0    |
| 295.00 | 473.0    |
| 296.00 | 20088.0  |
| 297.00 | 2513.0   |
| 298.00 | 183.0    |
| 301.00 | 309.0    |
| 302.00 | 368.0    |
| 303.10 | 2107.0   |
| 304.10 | 645.0    |
| 305.10 | 153.0    |
| 308.00 | 273.0    |
| 309.00 | 245.0    |
| 310.00 | 220.0    |
| 312.90 | 198.0    |
| 314.10 | 1083.0   |
| 315.00 | 2413.0   |
| 316.10 | 1083.0   |
| 317.10 | 259.0    |
| 321.00 | 694.0    |
| 321.90 | 294.0    |
| 323.10 | 6338.0   |
| 324.10 | 1172.0   |
| 327.00 | 1172.0   |
| 328.00 | 647.0    |
| 332.10 | 467.0    |
| 333.10 | 782.0    |
| 334.10 | 4169.0   |
| 335.10 | 1019.0   |
| 341.00 | 687.0    |
| 341.90 | 158.0    |
| 346.00 | 1272.0   |
| 347.00 | 203.0    |
| 352.10 | 1657.0   |
| 353.10 | 1131.0   |
| 354.10 | 2087.0   |
| 355.00 | 477.0    |
| 359.10 | 155.0    |
| 365.00 | 9738.0   |
| 366.00 | 1595.0   |
| 370.10 | 151.0    |
| 371.00 | 541.0    |
| 372.10 | 3516.0   |
| 373.10 | 864.0    |
| 383.00 | 1058.0   |
| 384.10 | 319.0    |
| 390.00 | 401.0    |
| 391.10 | 332.0    |
| 392.00 | 202.0    |
| 401.00 | 210.0    |
| 402.00 | 1413.0   |
| 403.00 | 1905.0   |
| 404.00 | 741.0    |
| 421.10 | 1919.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP025

|        |          |
|--------|----------|
| 422.00 | 1712.0   |
| 423.10 | 11777.0  |
| 424.10 | 3236.0   |
| 425.10 | 419.0    |
| 440.10 | 264.0    |
| 441.10 | 32248.0  |
| 442.10 | 213248.0 |
| 443.10 | 40336.0  |
| 444.10 | 3751.0   |
| 445.10 | 175.0    |

**Instrument :**  
BNA\_M  
**ClientSampleId :**  
DFTPP025