
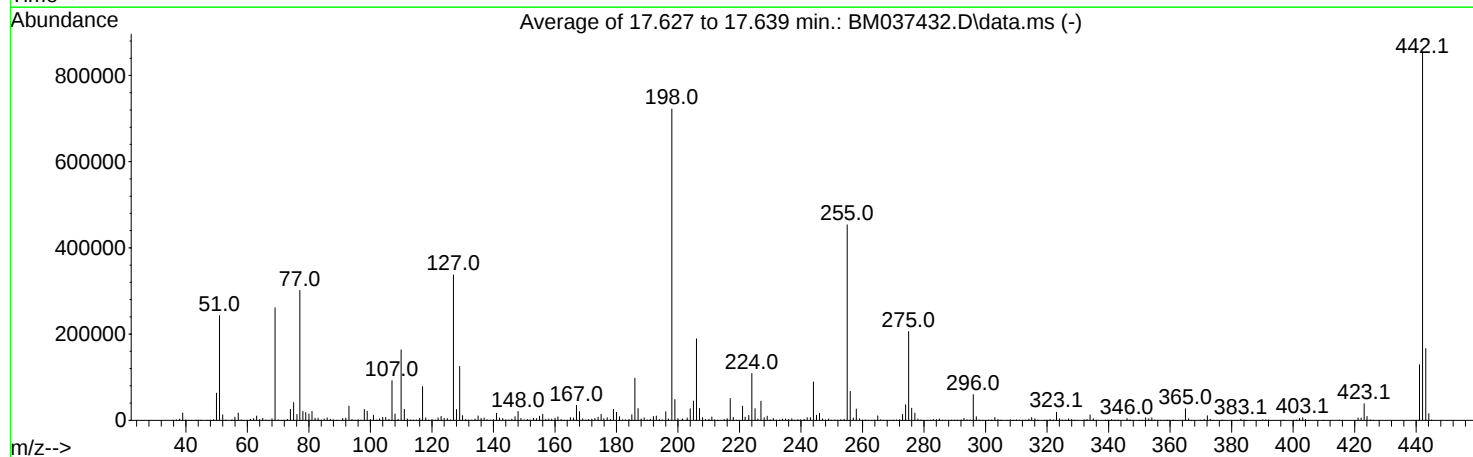


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110922\
Data File : BM037432.D
Acq On : 09 Nov 2022 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 09 02:08:14 2022

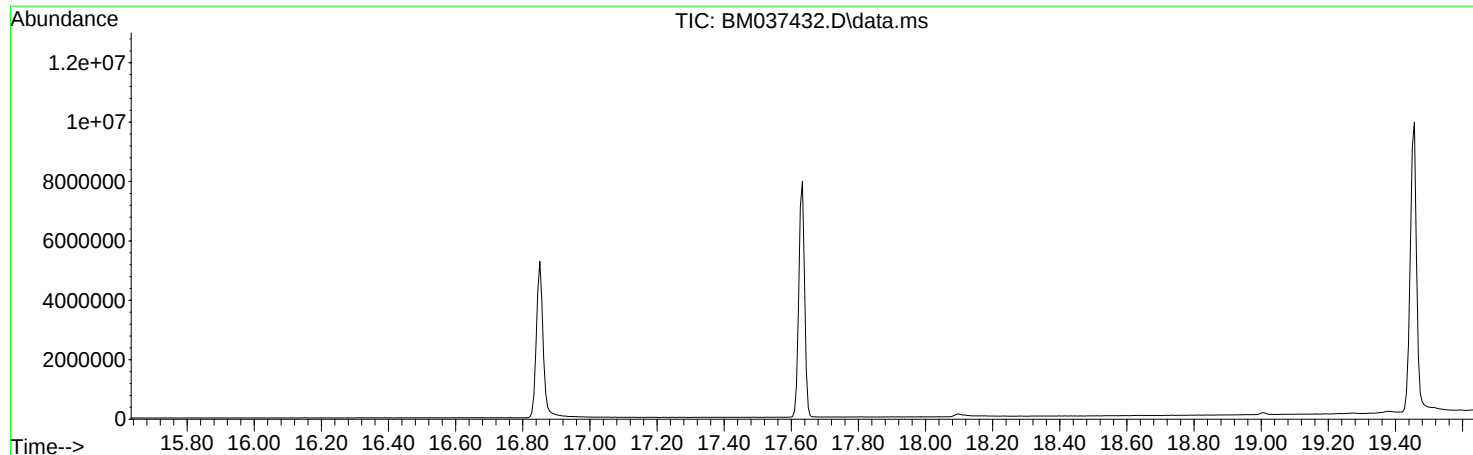




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	242917	PASS
68	69	0.00	2	1.3	3495	PASS
69	198	0.00	100	36.2	261269	PASS
70	69	0.00	2	0.4	1117	PASS
127	198	10	80	46.7	337429	PASS
197	198	0.00	2	0.4	3055	PASS
198	198	100	100	100.0	722133	PASS
199	198	5	9	6.6	47941	PASS
275	198	10	60	28.5	205995	PASS
365	198	1	100	3.7	26933	PASS
441	198	0.01	100	17.9	129091	PASS
442	442	50	100	100.0	853419	PASS
443	442	15	24	19.5	166485	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110922\
Data File : BM037432.D
Acq On : 09 Nov 2022 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 10 07:40:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 02:08:14 2022
Response via : Initial Calibration

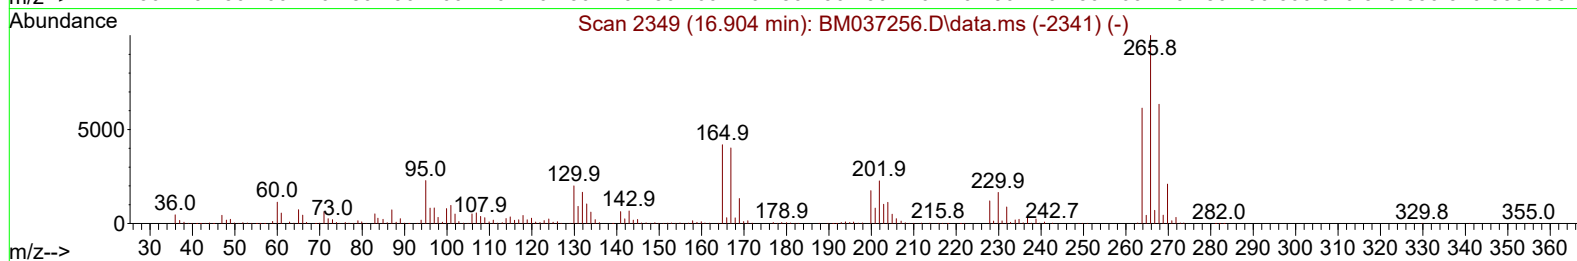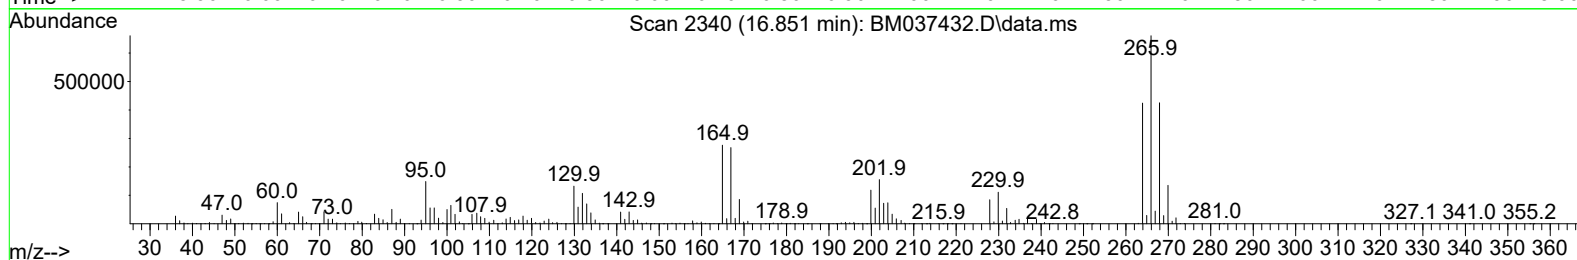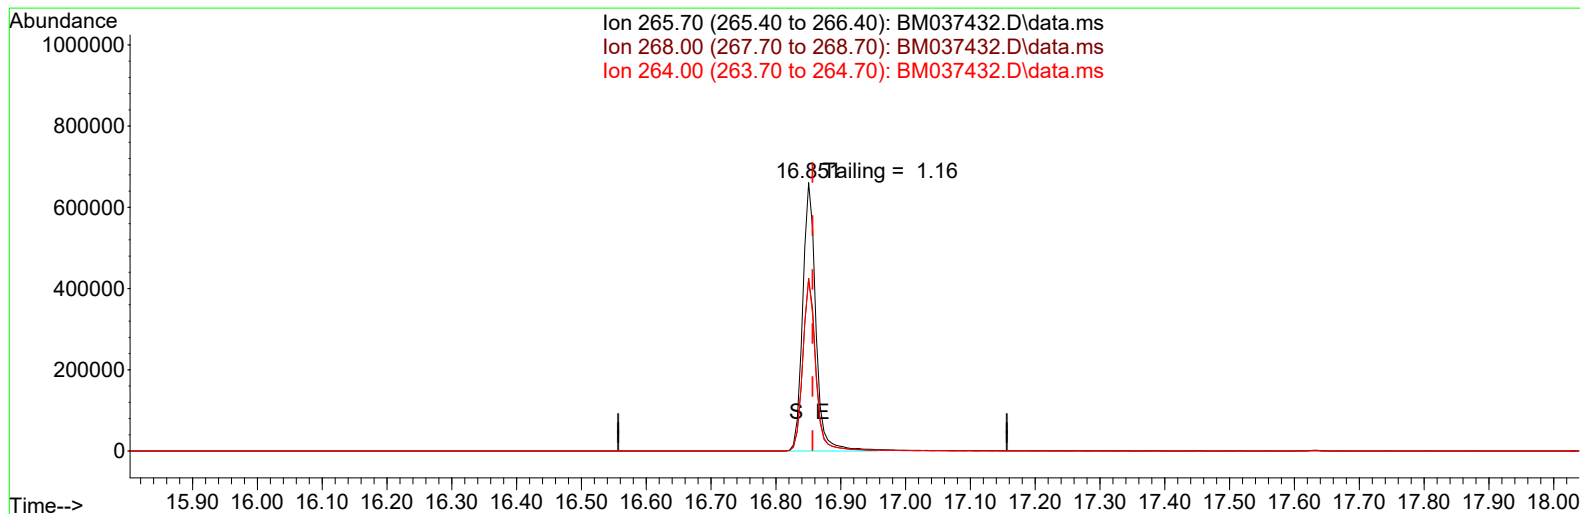

TIC: BM037432.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.006) 958029.83 ng

response 938770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.36
264.00	61.40	64.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2022	BNA_M	<u>BM037432.D</u>
Compound Name	Response	Retention Time
DDT	2761446	20.674
DDD	41525	20.28
DDE	3201	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44726	2806172	1.59

Instrument :
BNA_M
ClientSampleId :
DFTPP