

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111015\
 Data File : BM003081.D
 Acq On : 10 Nov 2015 17:38
 Operator : UM/IZ
 Sample : G4263-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YA280

Quant Time: Nov 13 10:45:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 02:32:24 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	6609	0.40	ng/ul	0.00
4) Naphthalene-d8	10.55	136	29864	0.40	ng/ul	0.00
5) Acenaphthene-d10	14.39	164	15295	0.40	ng/ul	-0.02
6) Phenanthrene-d10	17.13	188	36334	0.40	ng/ul	-0.01
7) Chrysene-d12	21.34	240	40772	0.40	ng/ul	0.00
8) Perylene-d12	23.60	264	33387	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.21	96	9327	1.45	ng/uL	-0.02
Target Compounds						
3) 1,4-Dioxane	3.24	88	1080	0.14	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111015\
Data File : BM003081.D
Acq On : 10 Nov 2015 17:38
Operator : UM/IZ
Sample : G4263-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YA280

Quant Time: Nov 13 10:45:29 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 02:32:24 2015
Response via : Initial Calibration

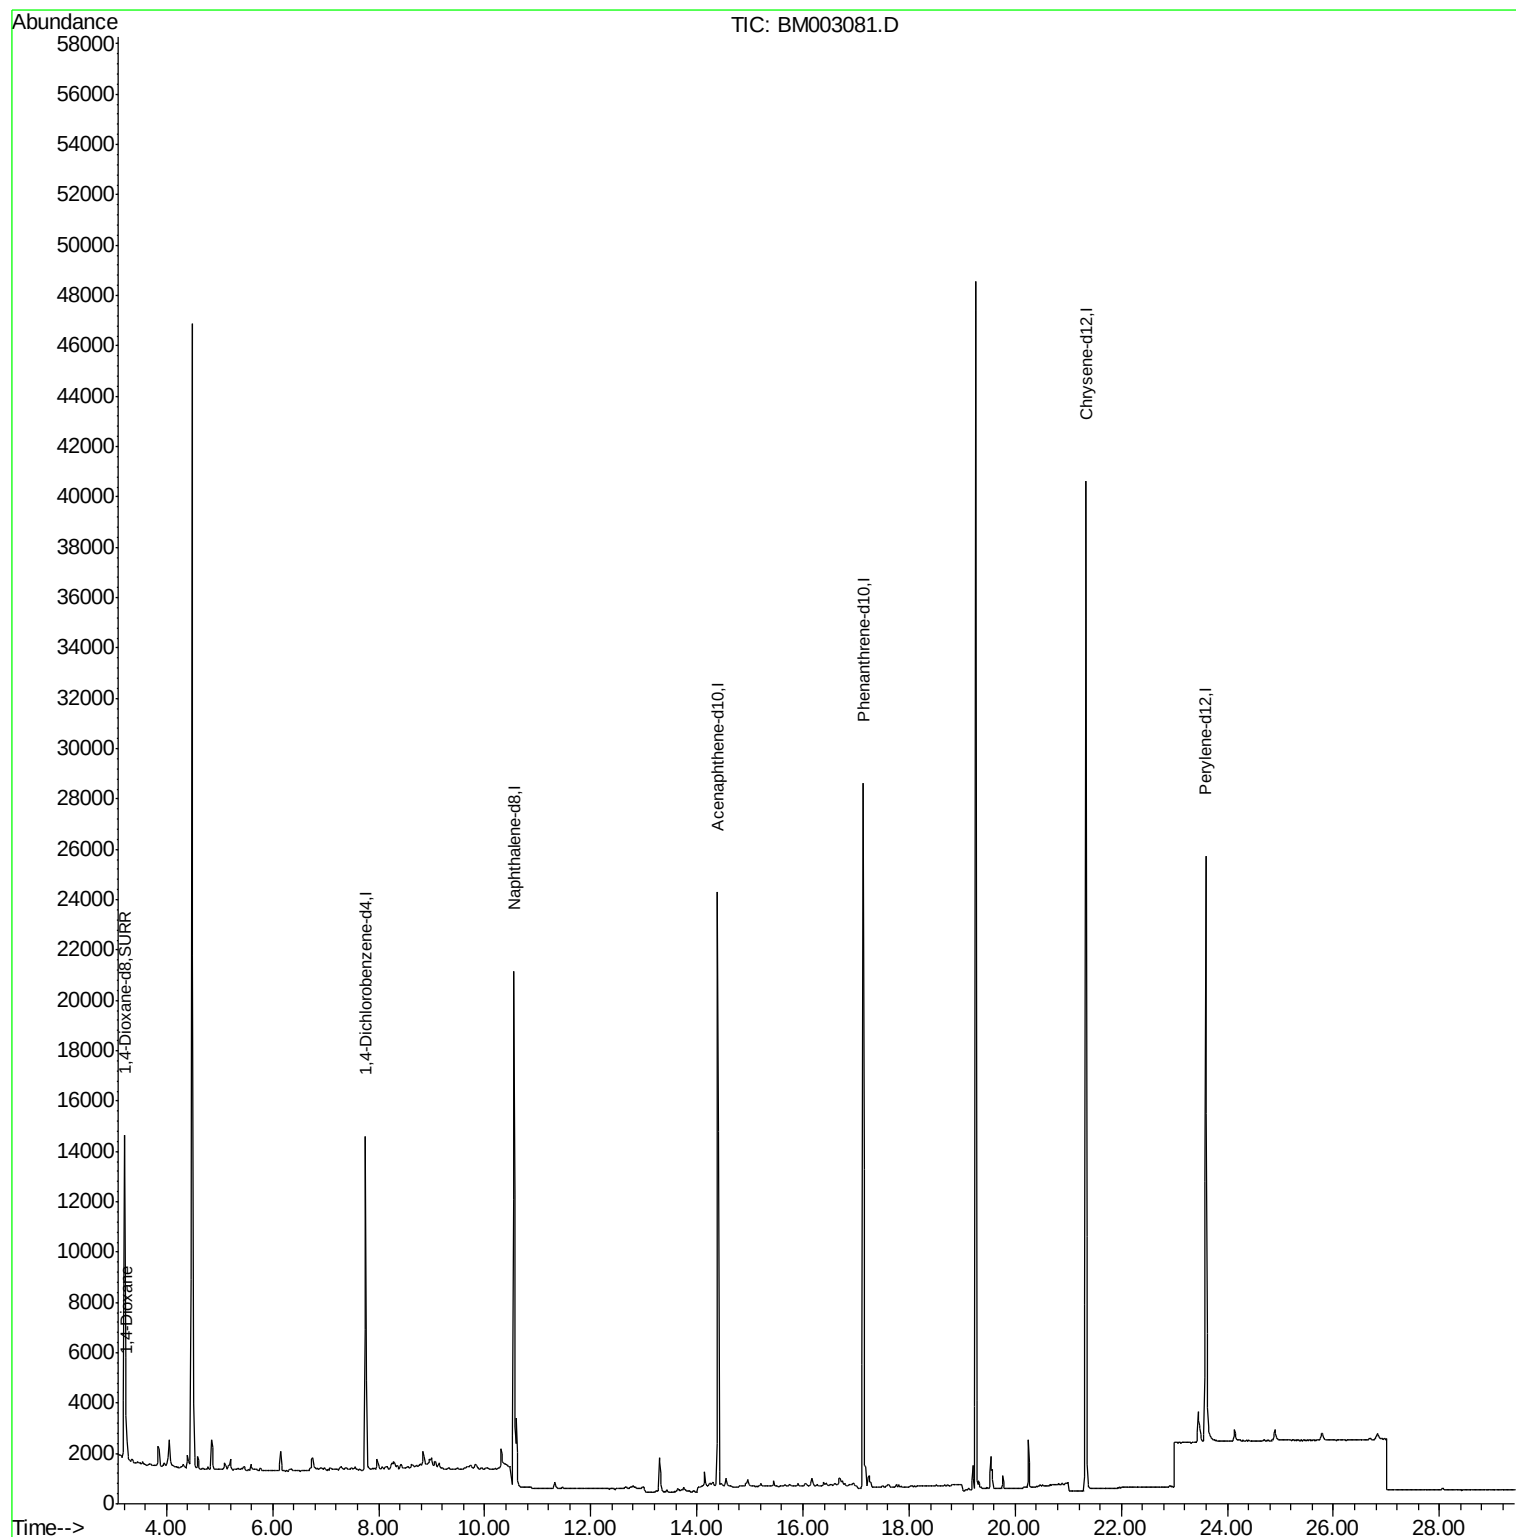

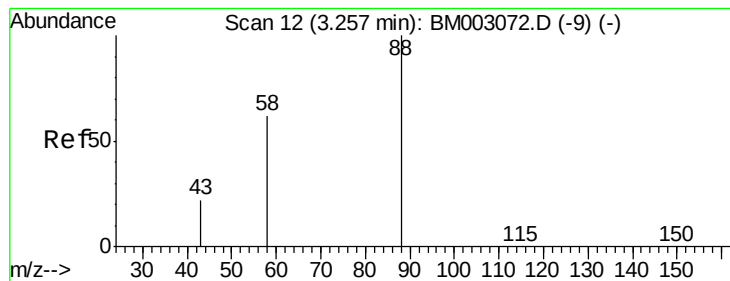

#3
 1,4-Dioxane
 Concen: 0.14 ng/ul
 RT: 3.24 min Scan# 11
 Delta R.T. -0.02 min
 Lab File: BM003081.D
 Acq: 10 Nov 2015 17:38

Instrument :
 BNA_M
 ClientSampleId :
 YA280

Tgt Ion: 88 Resp: 1080
 Ion Ratio Lower Upper
 88 100
 58 56.5 54.8 82.2
 43 35.3 22.6 33.8#

