

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111015\
 Data File : BM003083.D
 Acq On : 10 Nov 2015 18:50
 Operator : UM/IZ
 Sample : SSTDCCC002
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD00240

Quant Time: Nov 13 10:45:37 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 02:32:24 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	6985	0.40	ng/ul	0.00
4) Naphthalene-d8	10.55	136	29947	0.40	ng/ul	0.00
5) Acenaphthene-d10	14.39	164	14116	0.40	ng/ul	-0.02
6) Phenanthrene-d10	17.13	188	30946	0.40	ng/ul	-0.02
7) Chrysene-d12	21.34	240	25916	0.40	ng/ul	0.00
8) Perylene-d12	23.60	264	19085	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.21	96	13080	1.92	ng/uL	-0.02
Target Compounds						
3) 1,4-Dioxane	3.24	88	15049	1.85	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111015\
Data File : BM003083.D
Acq On : 10 Nov 2015 18:50
Operator : UM/IZ
Sample : SSTDCCC002
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD00240

Quant Time: Nov 13 10:45:37 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 02:32:24 2015
Response via : Initial Calibration

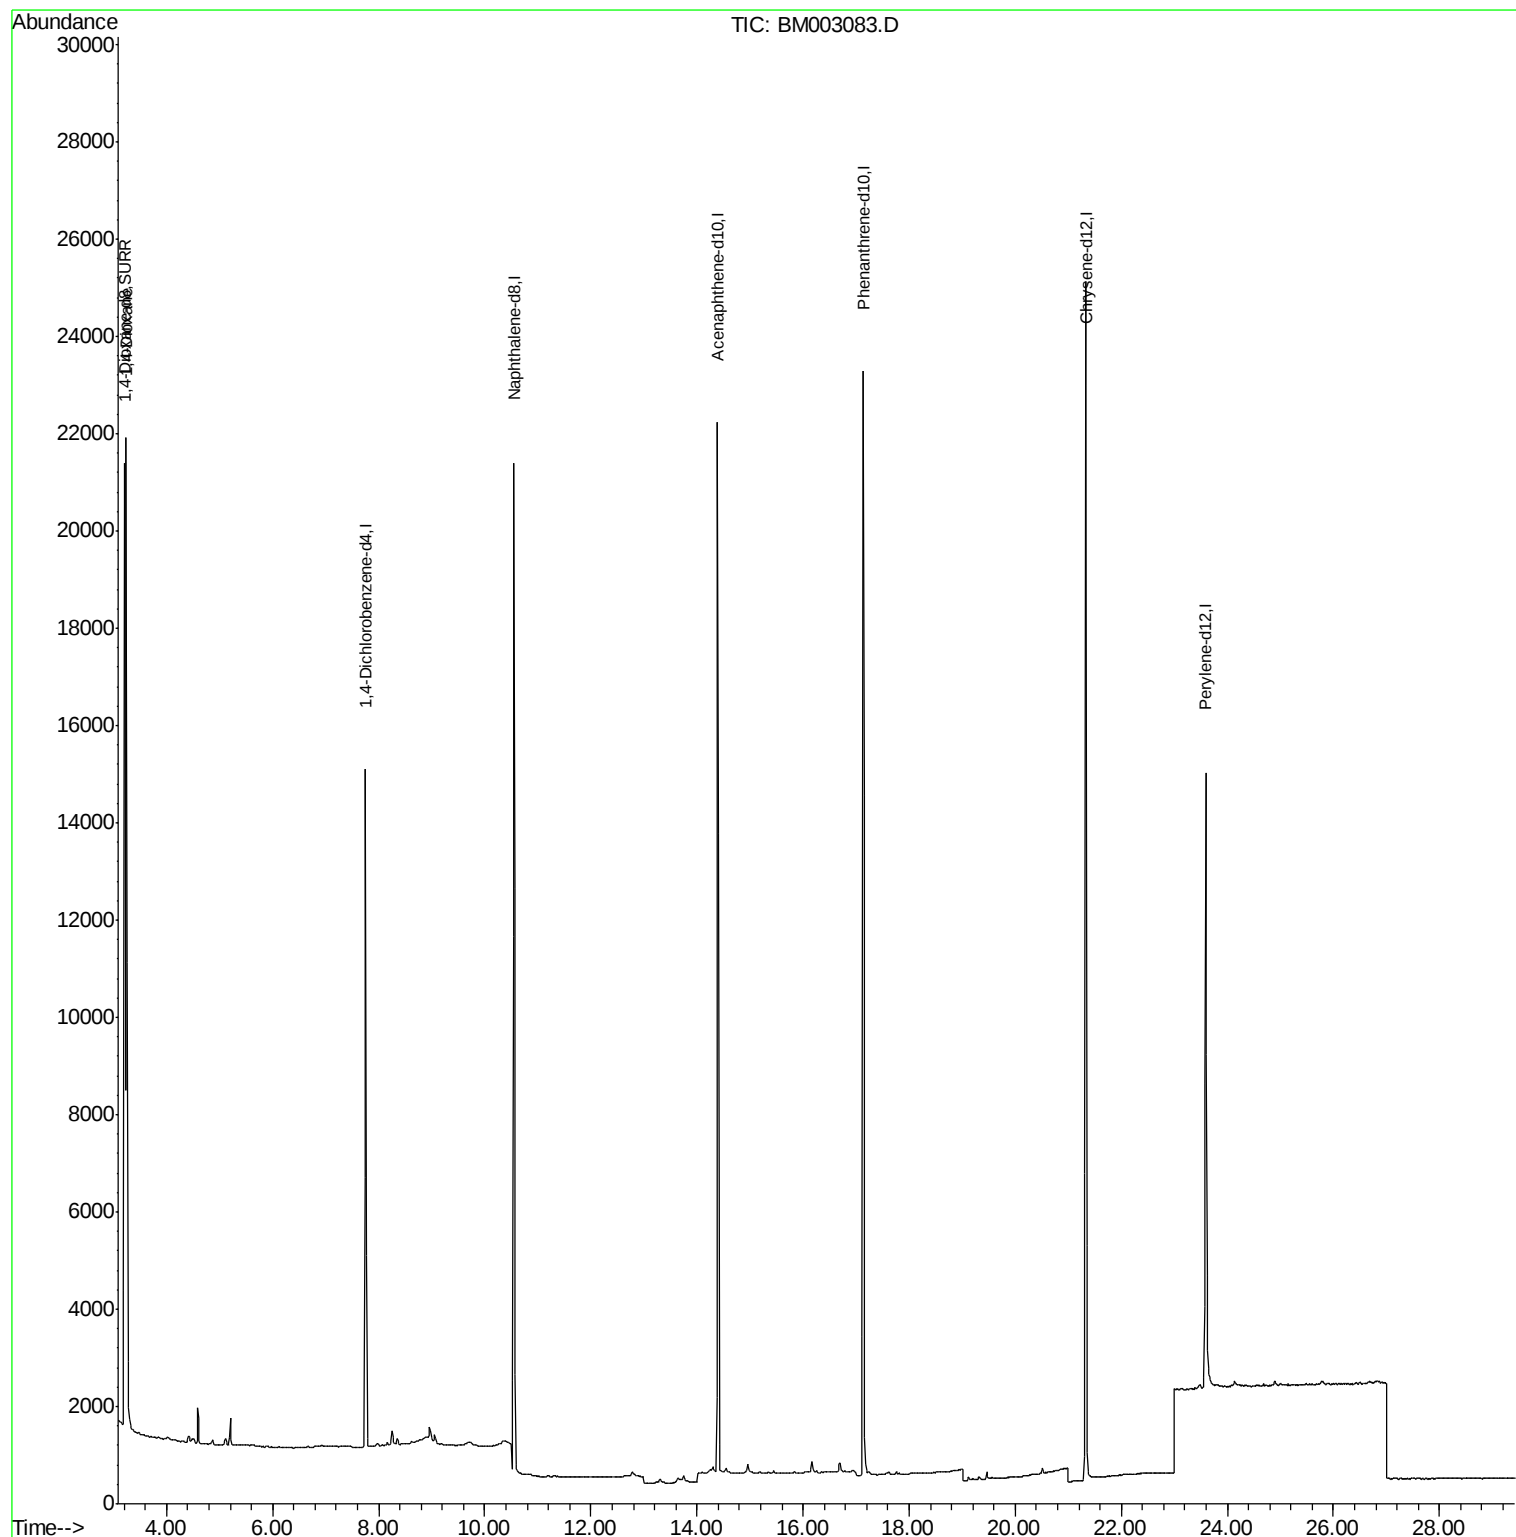

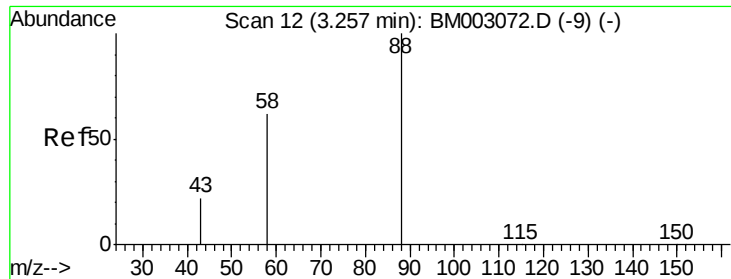

#3

1,4-Dioxane

Concen: 1.85 ng/ul

RT: 3.24 min Scan# 11

Delta R.T. -0.02 min

Lab File: BM003083.D

Acq: 10 Nov 2015 18:50

Instrument :

BNA_M

ClientSampleId :

SSTD00240

Tgt Ion: 88 Resp: 15049

Ion Ratio Lower Upper

88 100

58 70.4 54.8 82.2

43 29.5 22.6 33.8

