

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111015\
 Data File : BM003078.D
 Acq On : 10 Nov 2015 15:49
 Operator : UM/IZ
 Sample : PB86525BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS25

Quant Time: Nov 13 10:45:19 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 02:32:24 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	7415	0.40	ng/ul	0.00
4) Naphthalene-d8	10.55	136	31988	0.40	ng/ul	0.00
5) Acenaphthene-d10	14.39	164	15771	0.40	ng/ul	-0.02
6) Phenanthrene-d10	17.13	188	33867	0.40	ng/ul	-0.02
7) Chrysene-d12	21.34	240	29758	0.40	ng/ul	0.00
8) Perylene-d12	23.60	264	23448	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.21	96	9159	1.27	ng/uL	-0.02
Target Compounds						
3) 1,4-Dioxane	3.24	88	2936	0.34	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111015\
Data File : BM003078.D
Acq On : 10 Nov 2015 15:49
Operator : UM/IZ
Sample : PB86525BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS25

Quant Time: Nov 13 10:45:19 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-1,4-DIO SIM-BM110915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 02:32:24 2015
Response via : Initial Calibration

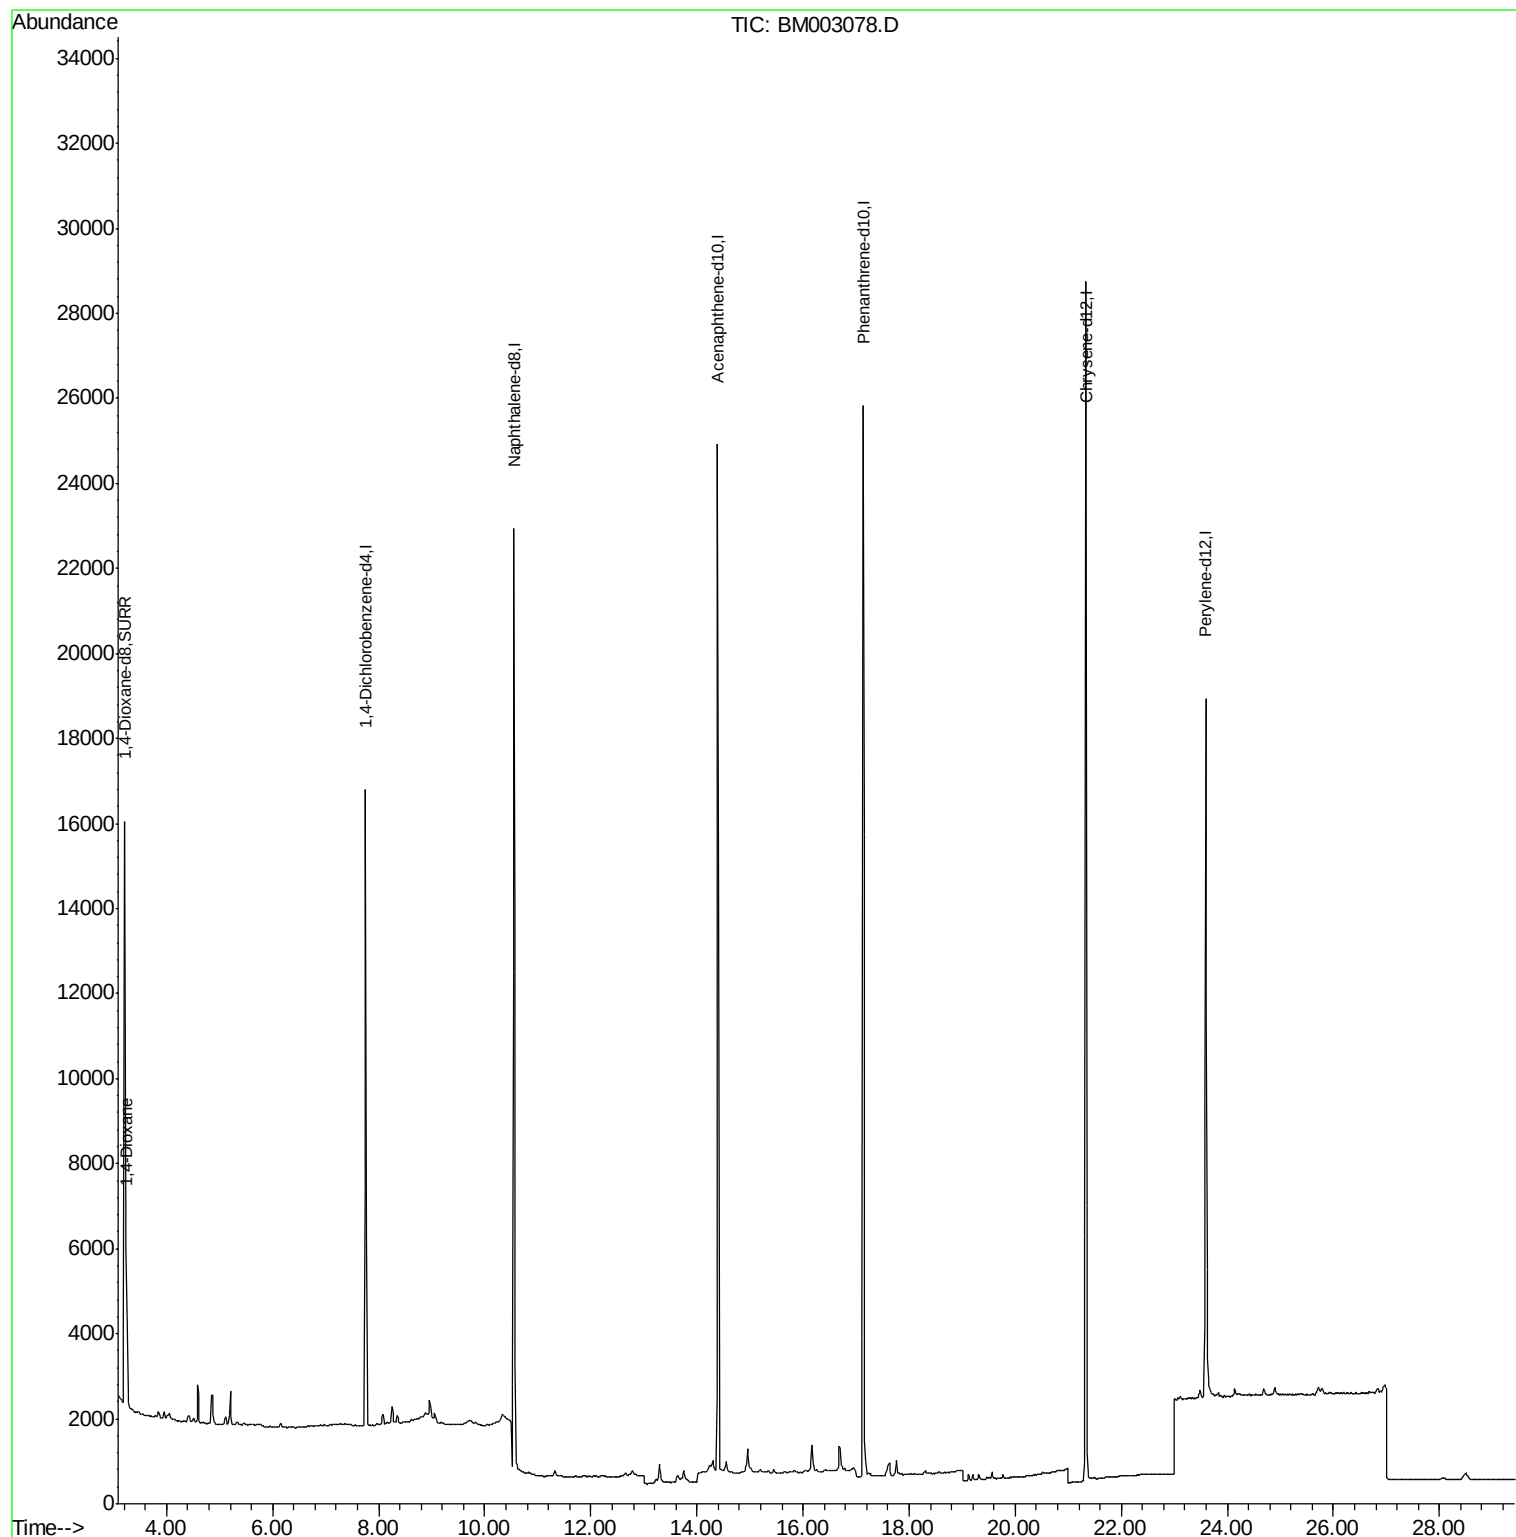

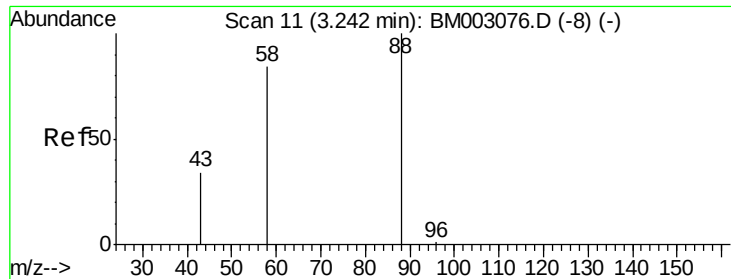

#3
 1,4-Dioxane
 Concen: 0.34 ng/ul
 RT: 3.24 min Scan# 11
 Delta R.T. -0.02 min
 Lab File: BM003078.D
 Acq: 10 Nov 2015 15:49

Instrument :
 BNA_M
 ClientSampleId :
 SLCS25

Tgt Ion: 88 Resp: 2936
 Ion Ratio Lower Upper
 88 100
 58 64.9 54.8 82.2
 43 29.8 22.6 33.8

