

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111017\
 Data File : BM012906.D
 Acq On : 11 Nov 2017 17:38
 Operator : SJ/JU
 Sample : I6322-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 13 01:10:10 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111017MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 13 01:07:29 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	67056	20.00	ng/ul	0.00
2) Naphthalene-d8	10.57	136	259888	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	159714	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.17	188	383837	20.00	ng/ul	0.00
17) Chrysene-d12	21.35	240	481613	20.00	ng/ul	0.00
22) Perylene-d12	23.63	264	526235	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.12	160	349801	21.06	ng/ul	0.00
10) Fluorene-d10	15.42	176	262738	23.12	ng/ul	0.00
14) Anthracene-d10	17.27	188	415133	22.37	ng/ul	0.00
18) Pyrene-d10	19.56	212	467427	21.69	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.48	264	546822	22.01	ng/ul	0.00
Target Compounds						
23) Benzo(b)fluoranthene	22.94	252	34167	1.09	ng/ul#	85
24) Benzo(k)fluoranthene	22.94	252	37062	1.24	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111017\
Data File : BM012906.D
Acq On : 11 Nov 2017 17:38
Operator : SJ/JU
Sample : I6322-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 13 01:10:10 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111017MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 13 01:07:29 2017
Response via : Initial Calibration




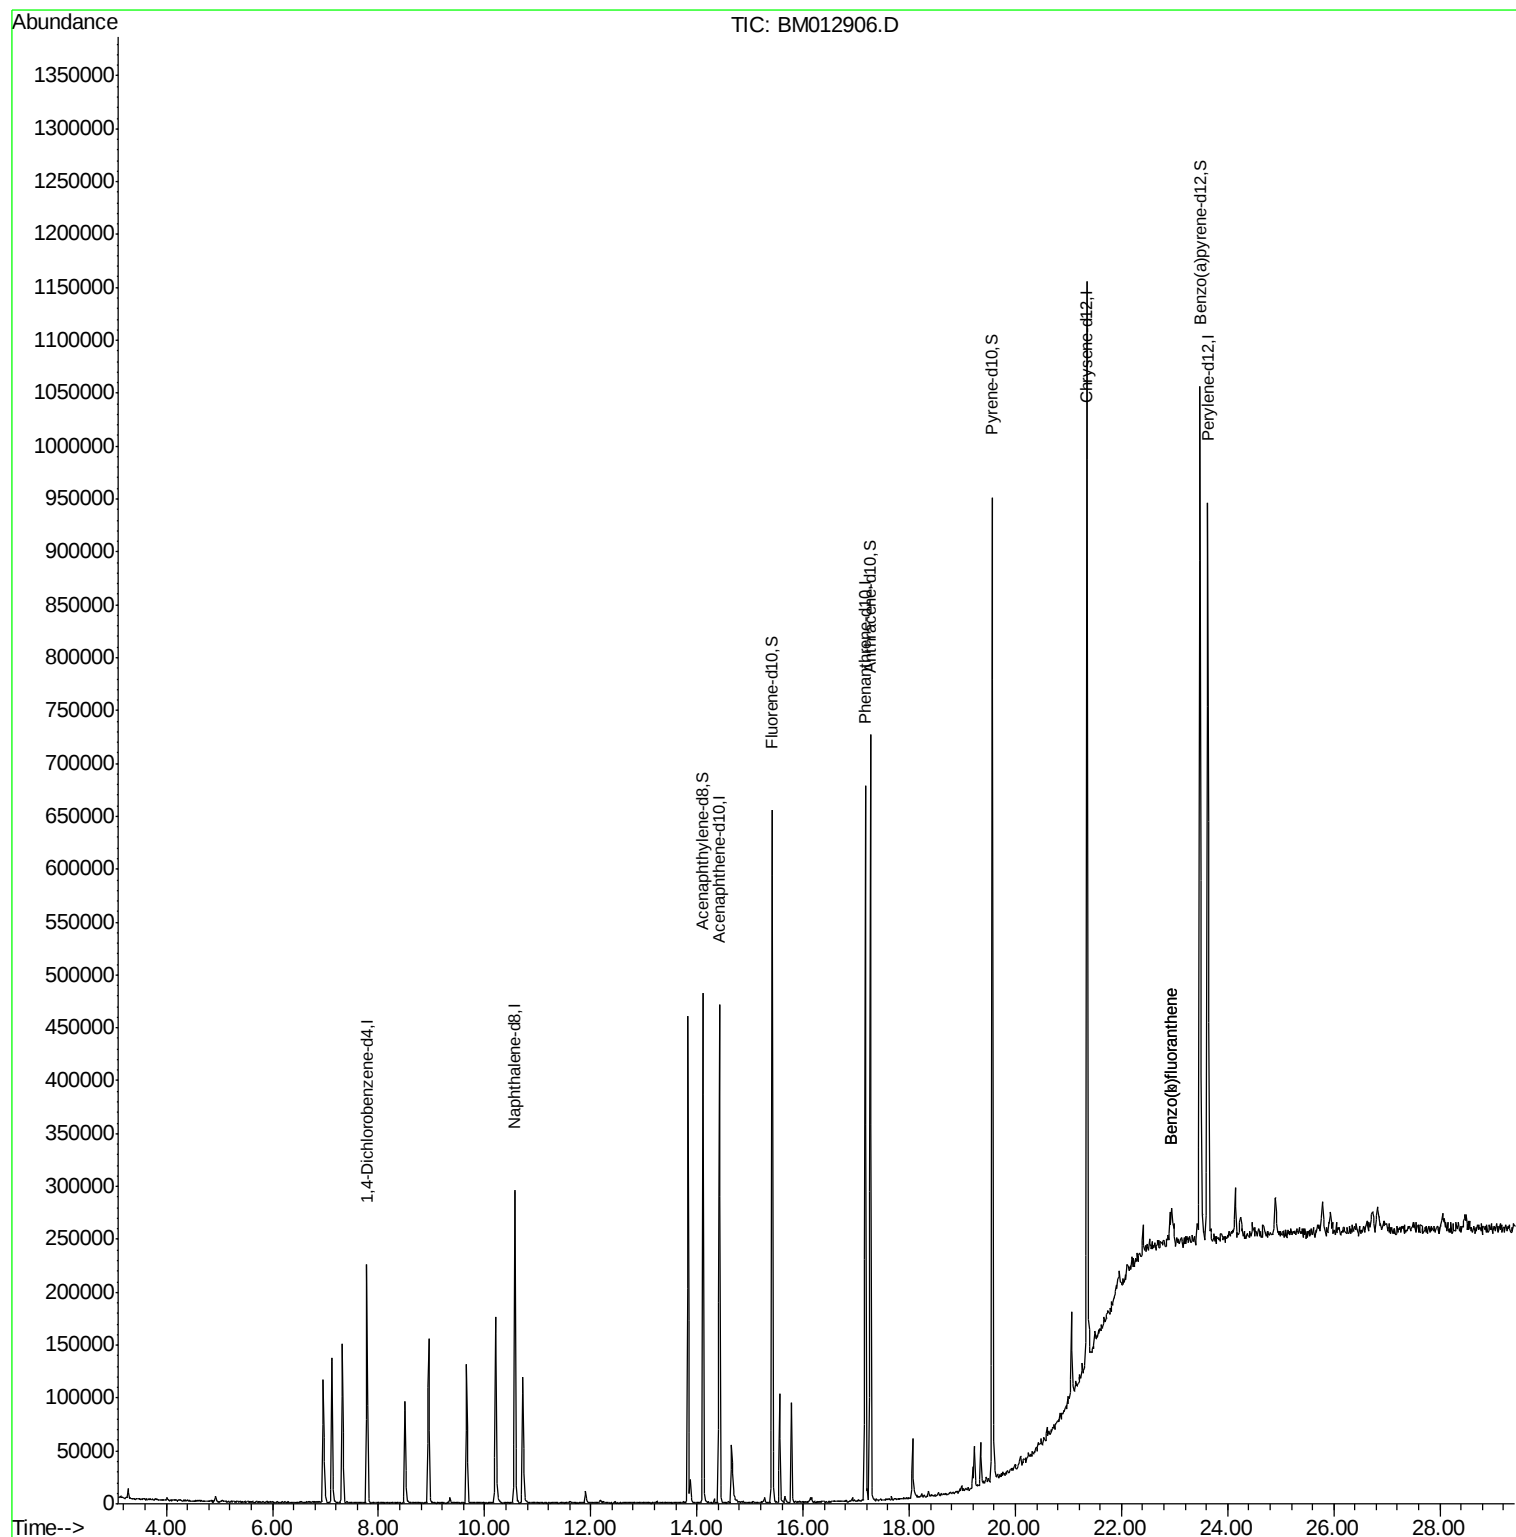


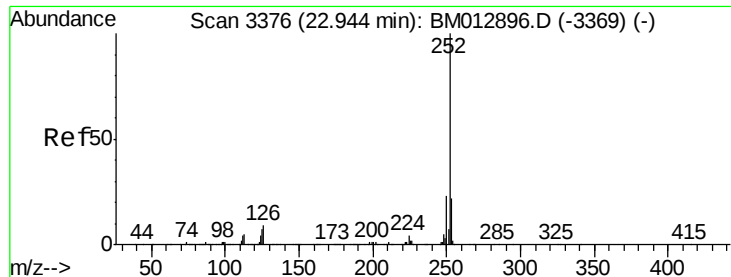

#23
Benzo(b)fluoranthene
Concen: 1.09 ng/ul
RT: 22.94 min Scan# 3376
Delta R.T. -0.00 min
Lab File: BM012906.D
Acq: 11 Nov 2017 17:38

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	30.7	18.0	27.0#
125	13.4	8.0	12.0#

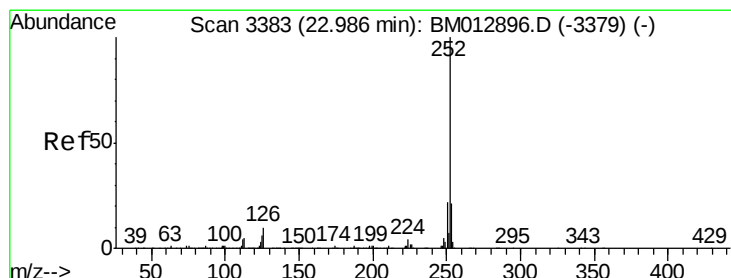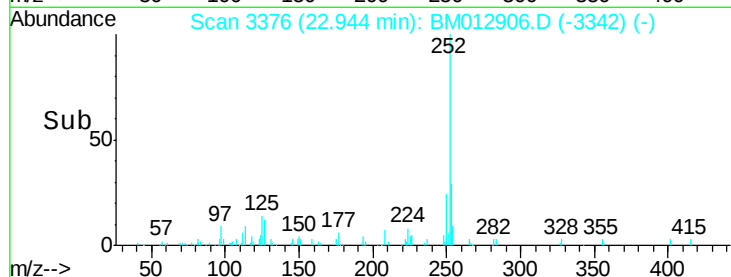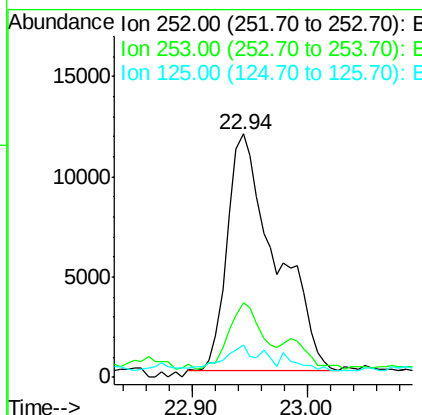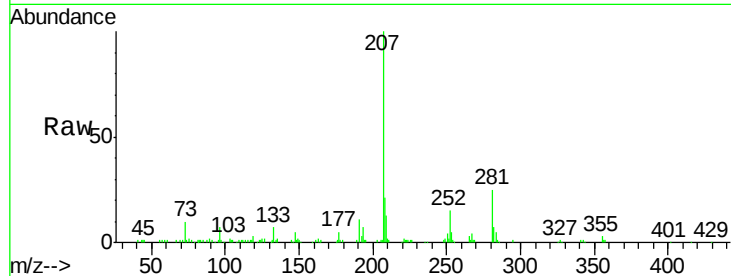

#24
Benzo(k)fluoranthene
Concen: 1.24 ng/ul
RT: 22.94 min Scan# 3376
Delta R.T. -0.04 min
Lab File: BM012906.D
Acq: 11 Nov 2017 17:38

Tgt Ion	Ratio	Lower	Upper
252	100		
253	30.7	18.0	27.0#
125	13.4	8.1	12.1#

