

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM111017\
 Data File : BM012916.D
 Acq On : 11 Nov 2017 23:33
 Operator : SJ/JU
 Sample : I6319-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAHNO

Manual Integrations
 APPROVED

SOHIL
 11/13/2017 4:49:48 PM

Quant Time: Nov 13 03:08:37 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111017MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 13 02:06:47 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	83078	20.00	ng/ul	0.00
2) Naphthalene-d8	10.57	136	314936	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	187199	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.17	188	439077	20.00	ng/ul	0.00
17) Chrysene-d12	21.35	240	539327	20.00	ng/ul	0.00
22) Perylene-d12	23.63	264	610477	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.12	160	436406	22.41	ng/ul	0.00
10) Fluorene-d10	15.42	176	314463	23.61	ng/ul	0.00
14) Anthracene-d10	17.27	188	484340	22.82	ng/ul	0.00
18) Pyrene-d10	19.56	212	579139	24.00	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.48	264	700025	24.29	ng/ul	0.00
Target Compounds						
23) Benzo(b)fluoranthene	22.94	252	52442m	1.445	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM111017\
Data File : BM012916.D
Acq On : 11 Nov 2017 23:33
Operator : SJ/JU
Sample : I6319-17
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DAHNO

Quant Time: Nov 13 03:08:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111017MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 13 02:06:47 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

SOHIL
11/13/2017 4:49:48 PM

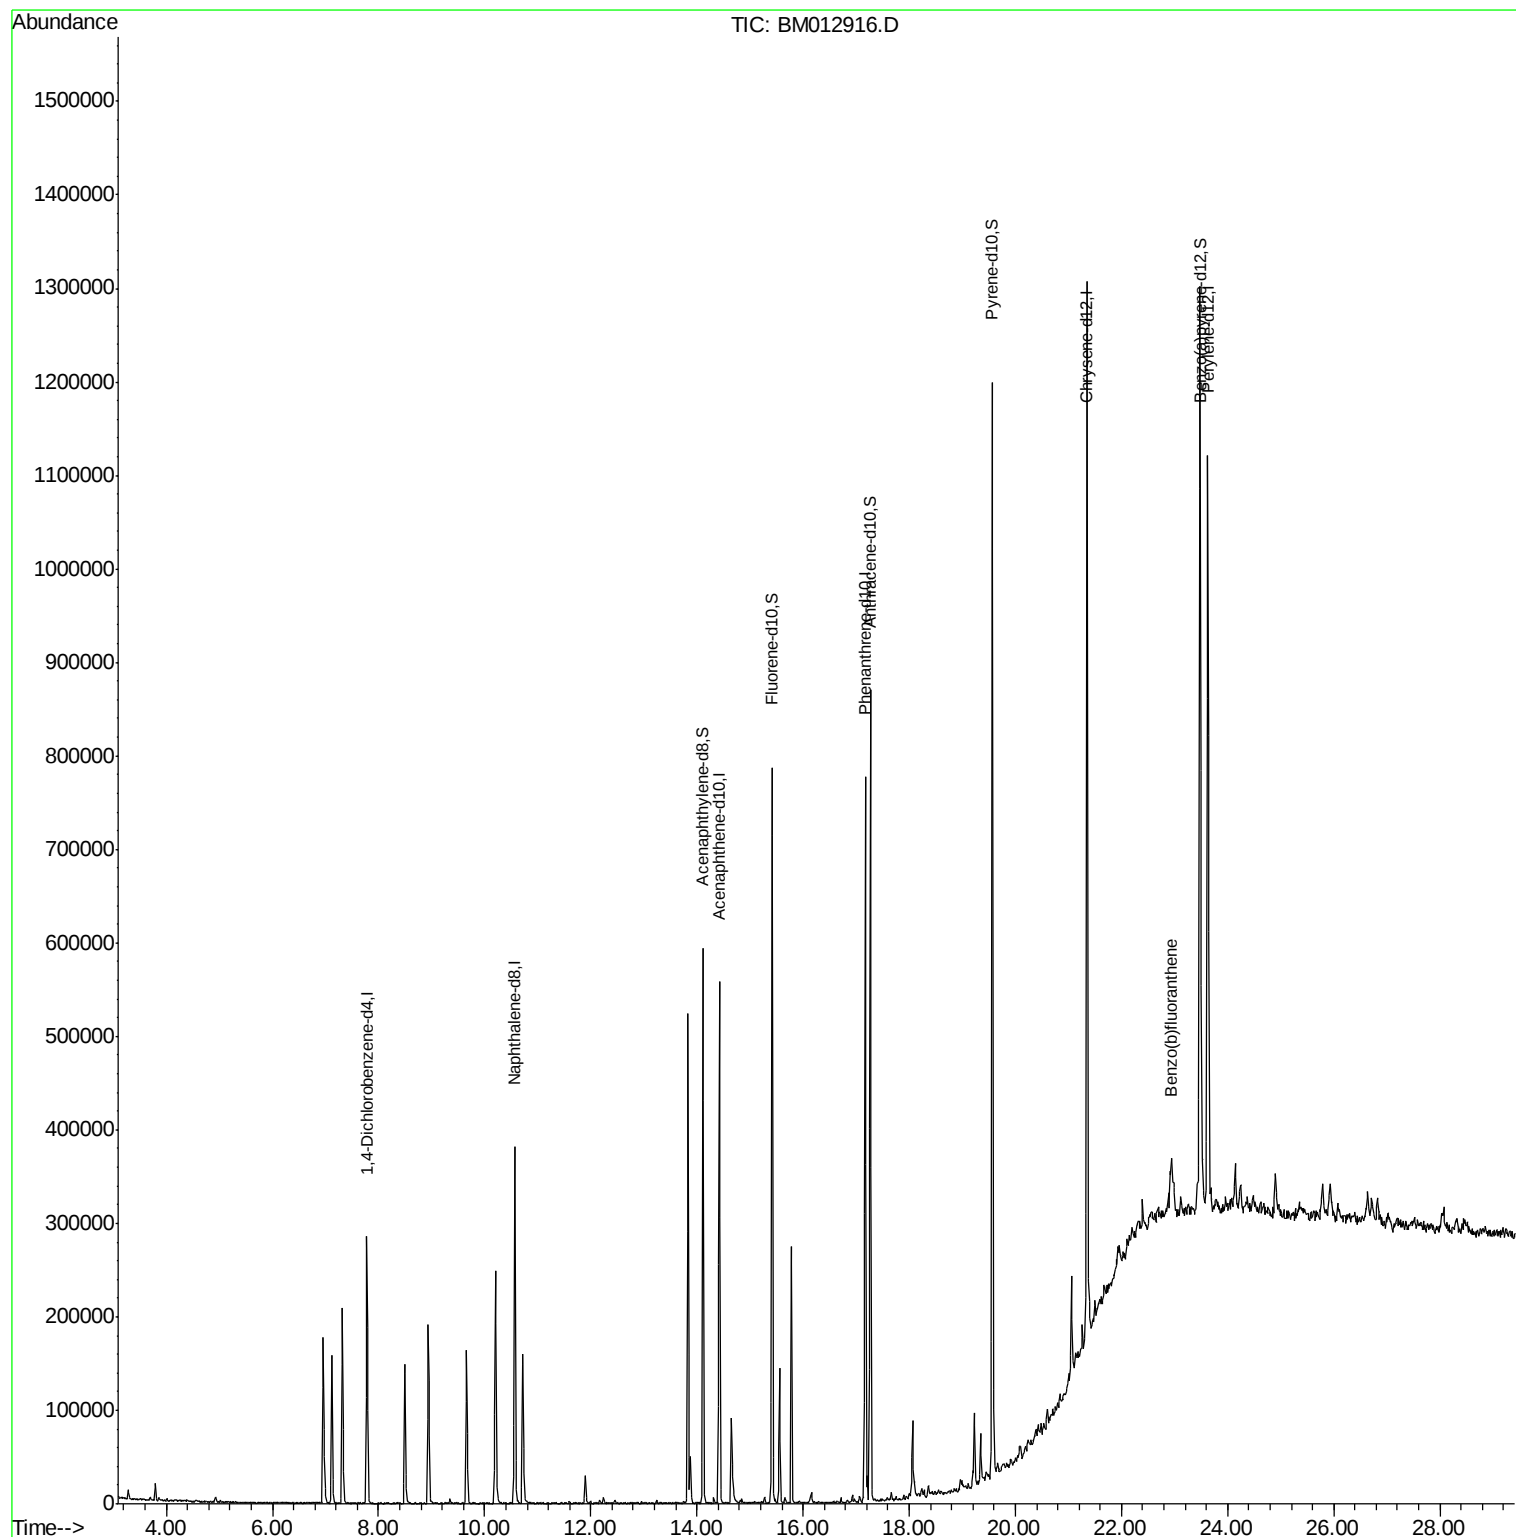

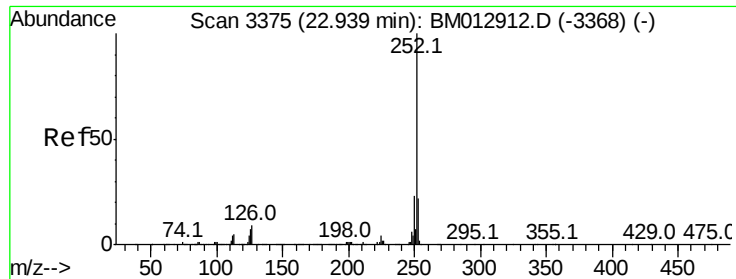

#23

Benzo(b)fluoranthene

Concen: 1.445 ng/ul m

RT: 22.94 min Scan# 3376

Delta R.T. 0.01 min

Lab File: BM012916.D


Acq: 11 Nov 2017 23:33

Instrument :

BNA_M

ClientSampleId :

DAHNO

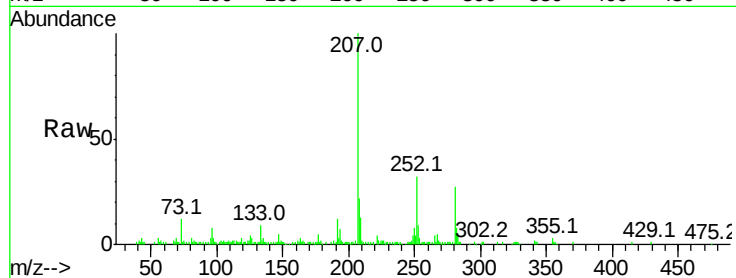

Tot Ion:	252	Resp:	52442
Ion Ratio	Lower	Upper	
252	100		
253	26.4	18.0	27.0
125	10.9	8.0	12.0

Manual Integrations
APPROVED

SOHIL
11/13/2017 4:49:48 PM

