
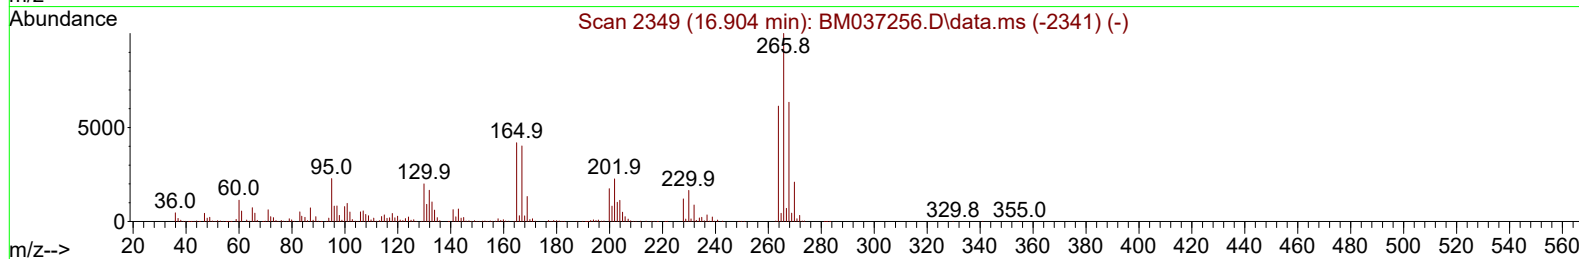
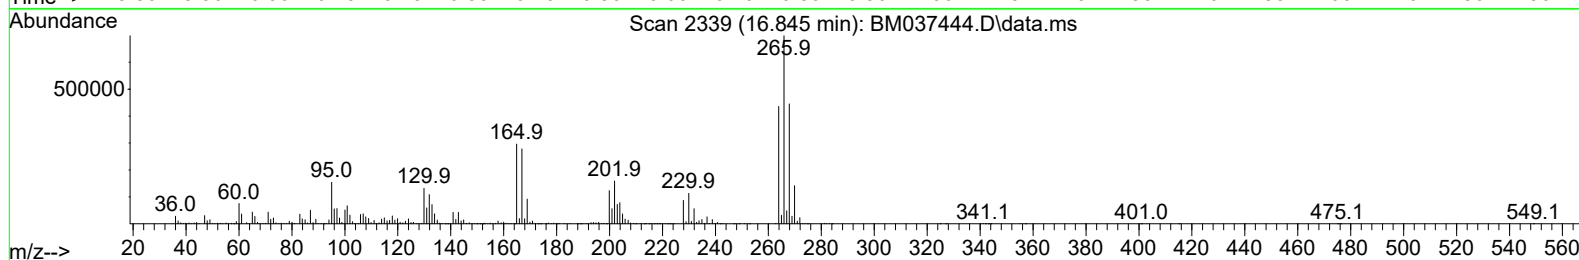


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\  
Data File : BM037444.D  
Acq On    : 10 Nov 2022  10:32  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 10 15:57:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 02:08:14 2022
Response via : Initial Calibration

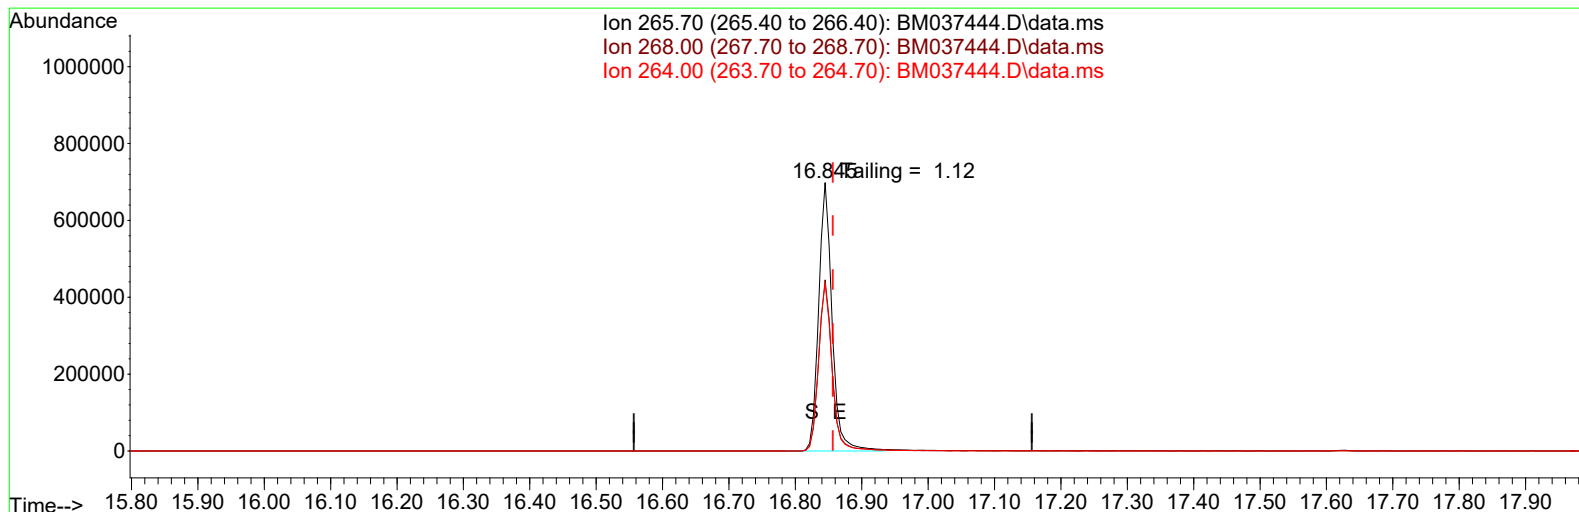

TIC: BM037444.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.012) 886032.28 ng

response **987250**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.72
264.00	61.40	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
 Data File : BM037444.D
 Acq On : 10 Nov 2022 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 15:57:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 09 02:08:14 2022
 Response via : Initial Calibration

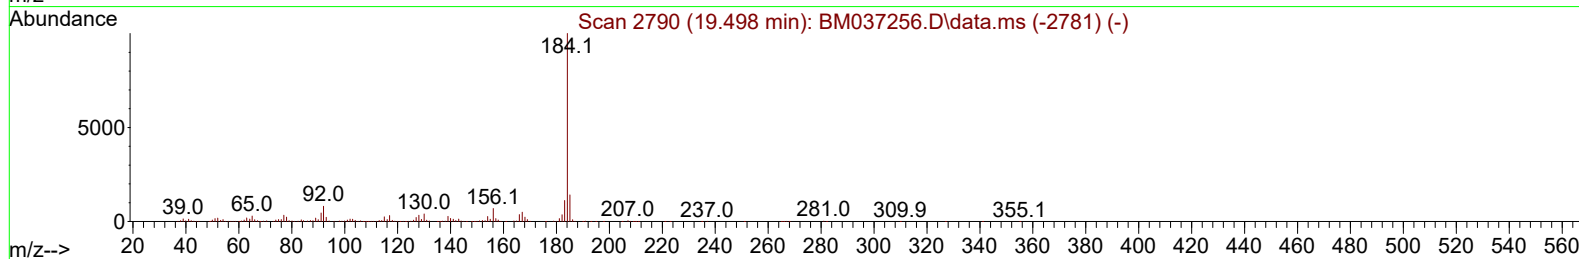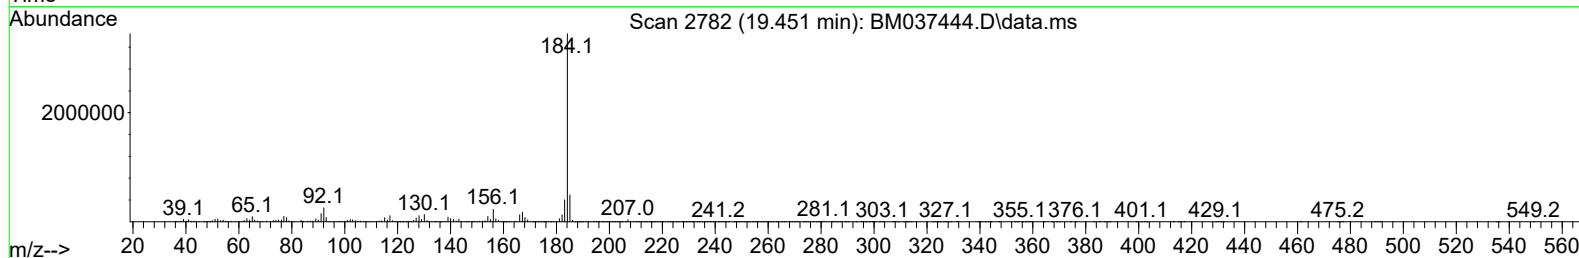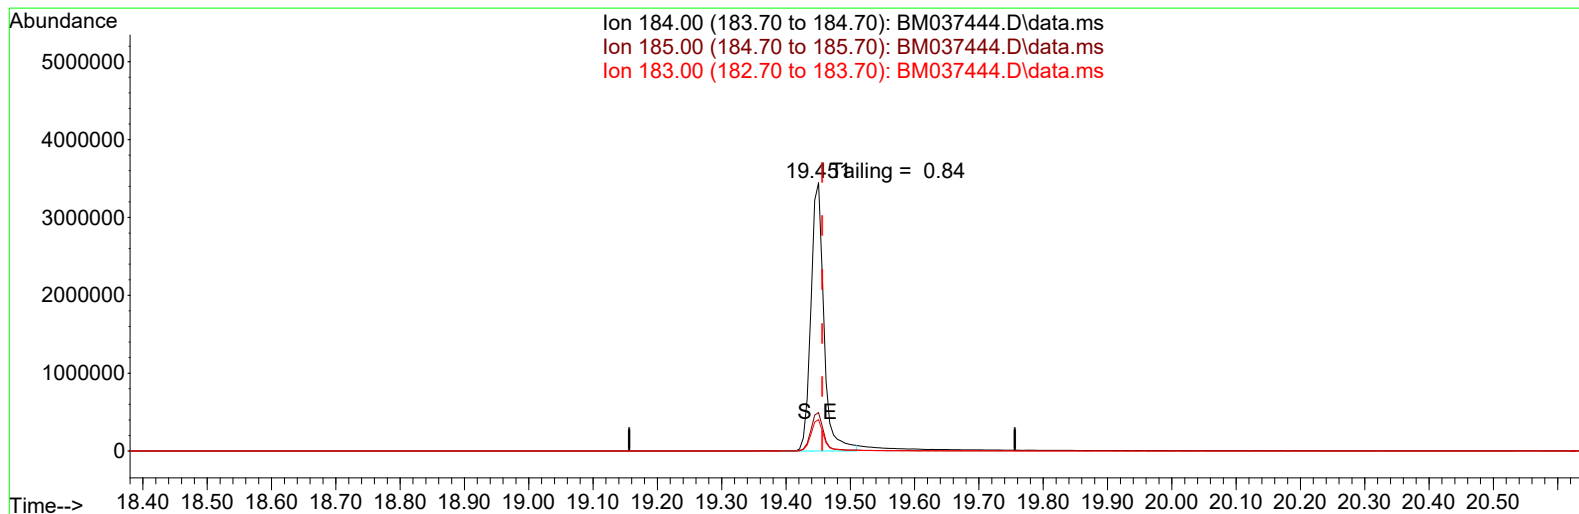

TIC: BM037444.D\data.ms

(77) Benzidine

19.451min (-0.006) 258618.52 ng

response 5113534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.34
183.00	11.20	11.71
0.00	0.00	0.00