

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
 Data File : BM037446.D
 Acq On : 10 Nov 2022 11:43
 Operator : CG/JU
 Sample : PB148920BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB148920BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM037446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.922	307	312	321	rBV	701547	958237	4.21%	1.018%
2	5.387	384	391	409	rBV	5679014	8037748	35.28%	8.543%
3	6.998	657	665	681	rBV	5516408	8592505	37.71%	9.132%
4	7.810	795	803	812	rBV	1170201	1799766	7.90%	1.913%
5	8.981	994	1002	1016	rBV	3202054	5360598	23.53%	5.697%
6	10.610	1268	1279	1299	rBV	1515924	2594910	11.39%	2.758%
7	13.075	1691	1698	1713	rBV	10197438	14410137	63.25%	15.315%
8	14.451	1925	1932	1945	rBV	2557915	3833063	16.82%	4.074%
9	15.939	2178	2185	2208	rBV	8861955	12633909	55.45%	13.427%
10	17.192	2392	2398	2411	rBV	3226531	4620576	20.28%	4.911%
11	18.092	2546	2551	2560	rBV2	93428	239521	1.05%	0.255%
12	19.815	2838	2844	2854	rBV	18291762	22784144	100.00%	24.215%
13	21.368	3104	3108	3117	rBV	3370385	4436829	19.47%	4.715%
14	23.697	3499	3504	3515	rVB2	1942788	3789150	16.63%	4.027%




Sum of corrected areas: 94091093

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
Data File : BM037446.D
Acq On : 10 Nov 2022 11:43
Operator : CG/JU
Sample : PB148920BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB148920BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

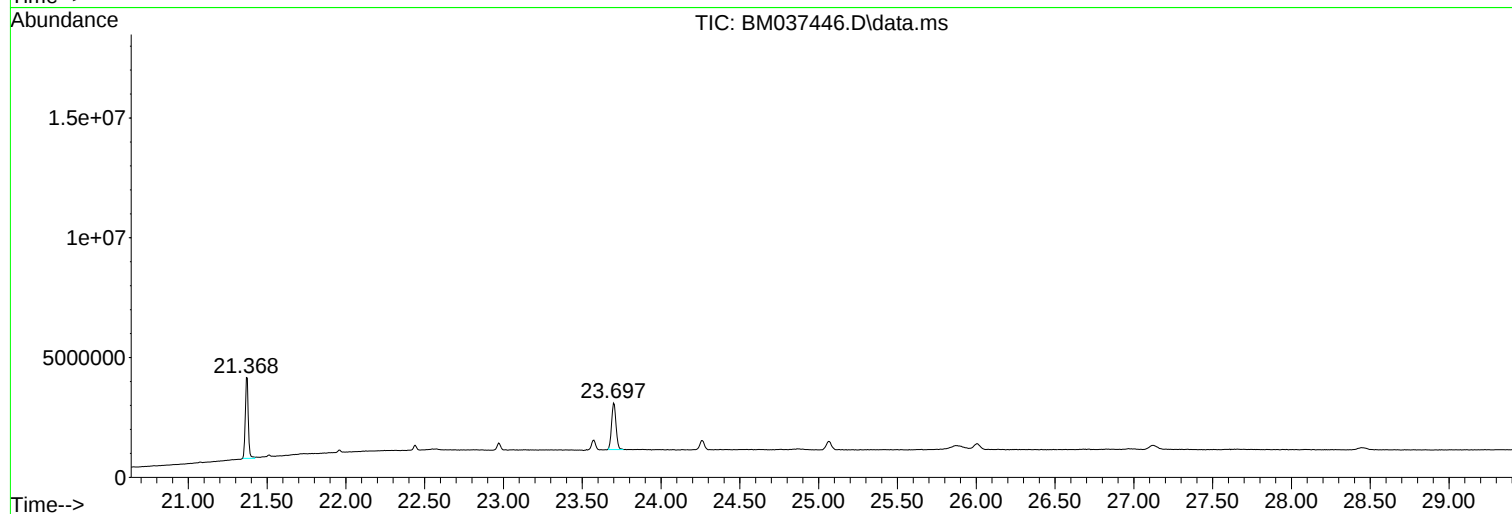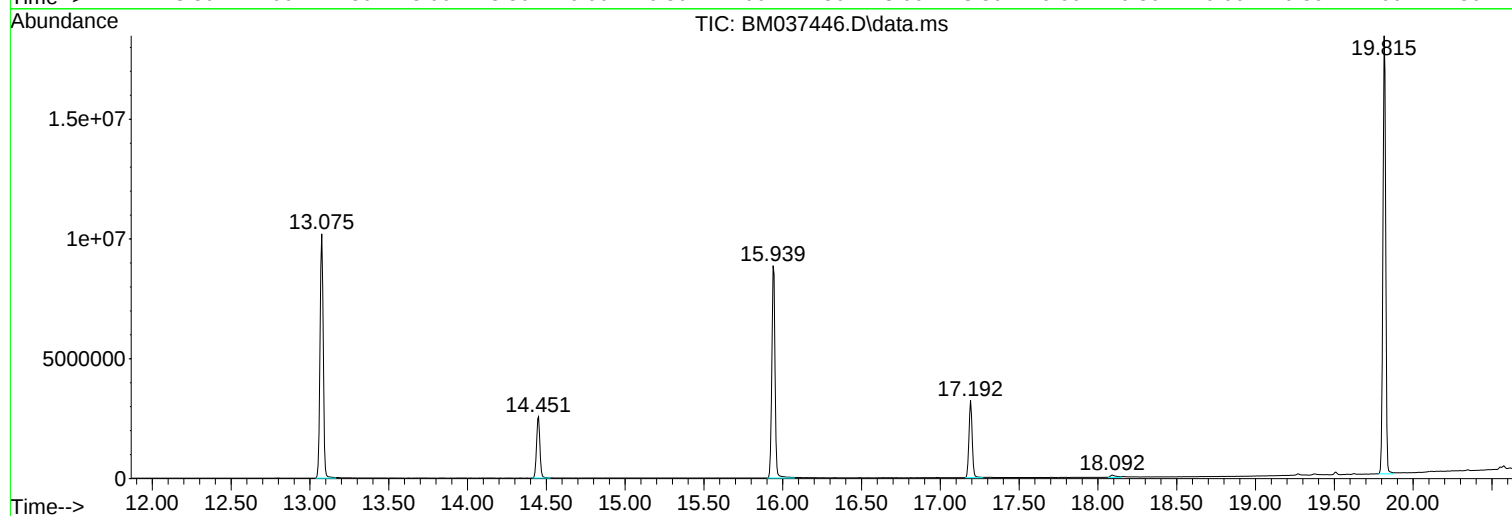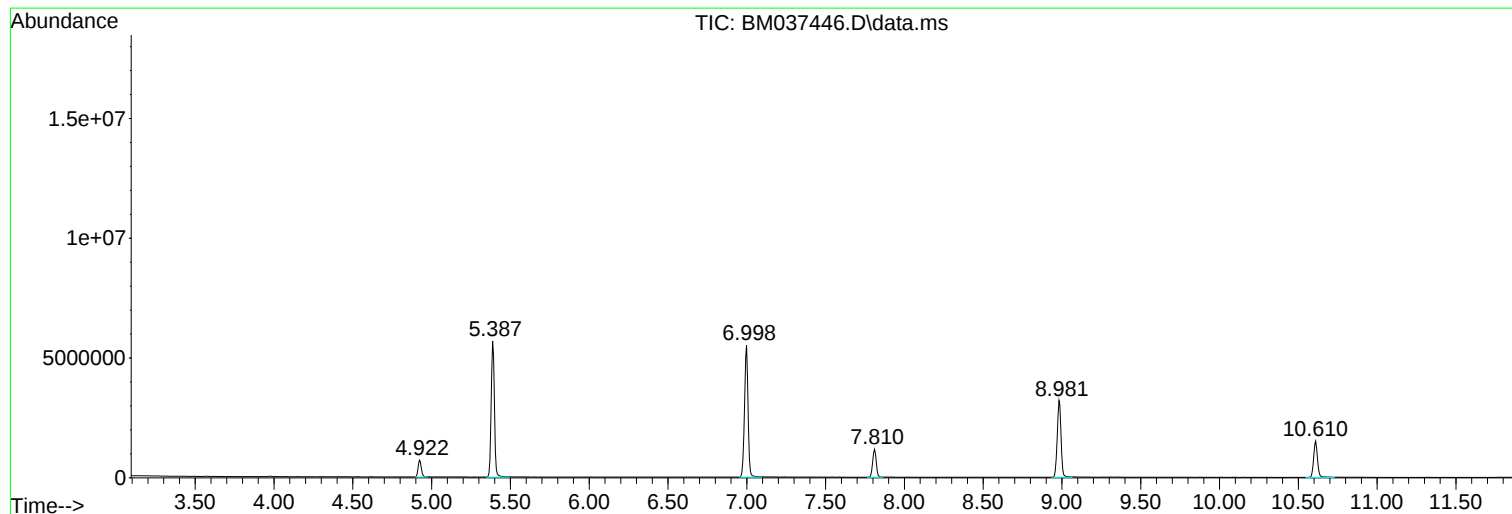

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
Data File : BM037446.D
Acq On : 10 Nov 2022 11:43
Operator : CG/JU
Sample : PB148920BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB148920BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.922	10.65 ng	958237	1,4-Dichlorobenzene-d4			7.810
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	50
2	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	25
3	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9
4	Morpholine, 4-methyl-		101	C5H11NO	000109-02-4	9
5	Butane, 1-ethoxy-		102	C6H14O	000628-81-9	9

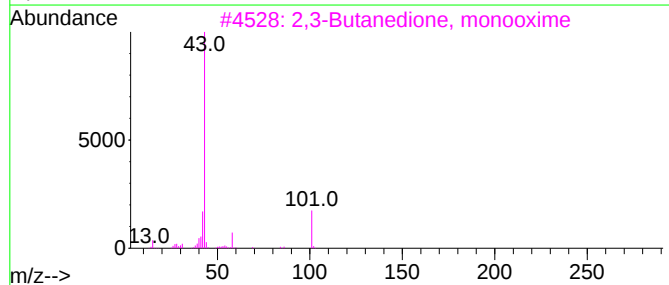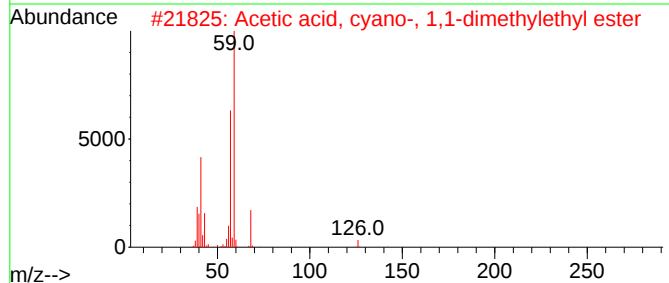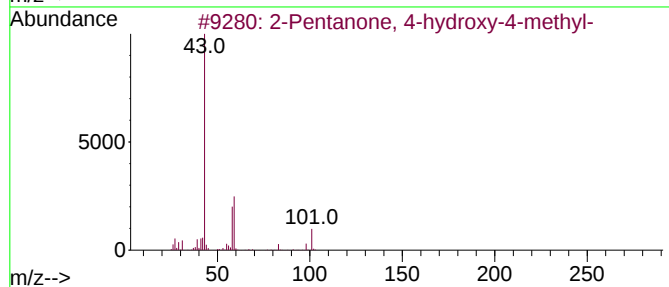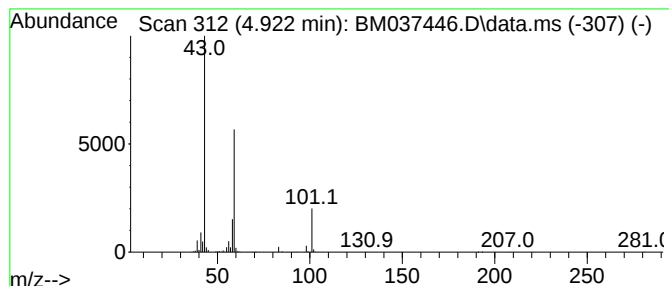

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
Data File : BM037446.D
Acq On : 10 Nov 2022 11:43
Operator : CG/JU
Sample : PB148920BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB148920BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.922	10.7	ng	958237	1	7.810	1799770	20.0