
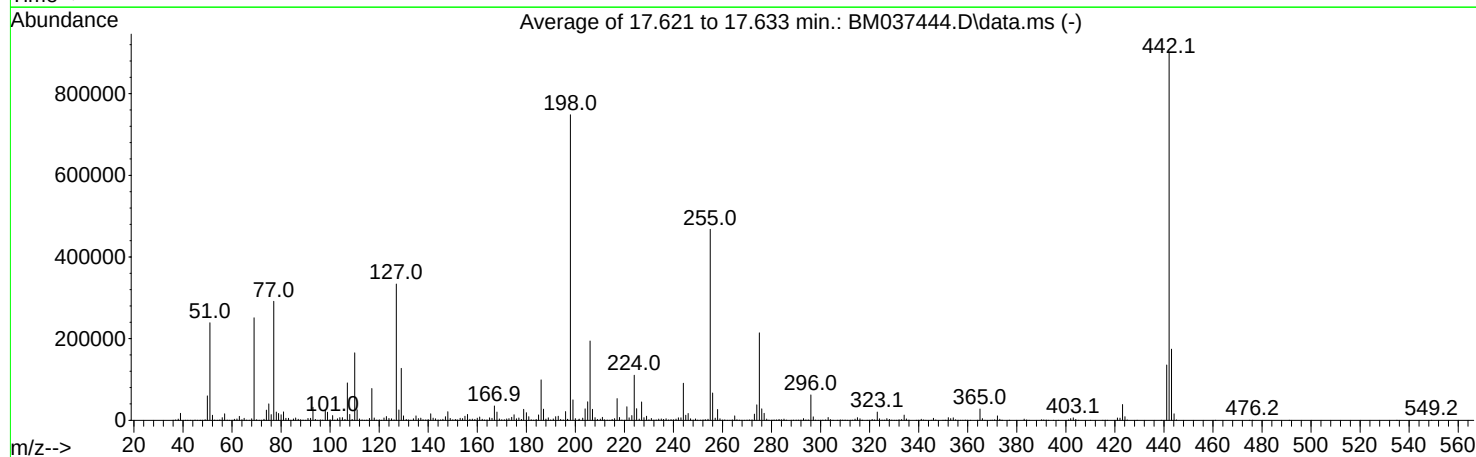


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
 Data File : BM037444.D
 Acq On : 10 Nov 2022 10:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 11 00:30:57 2022

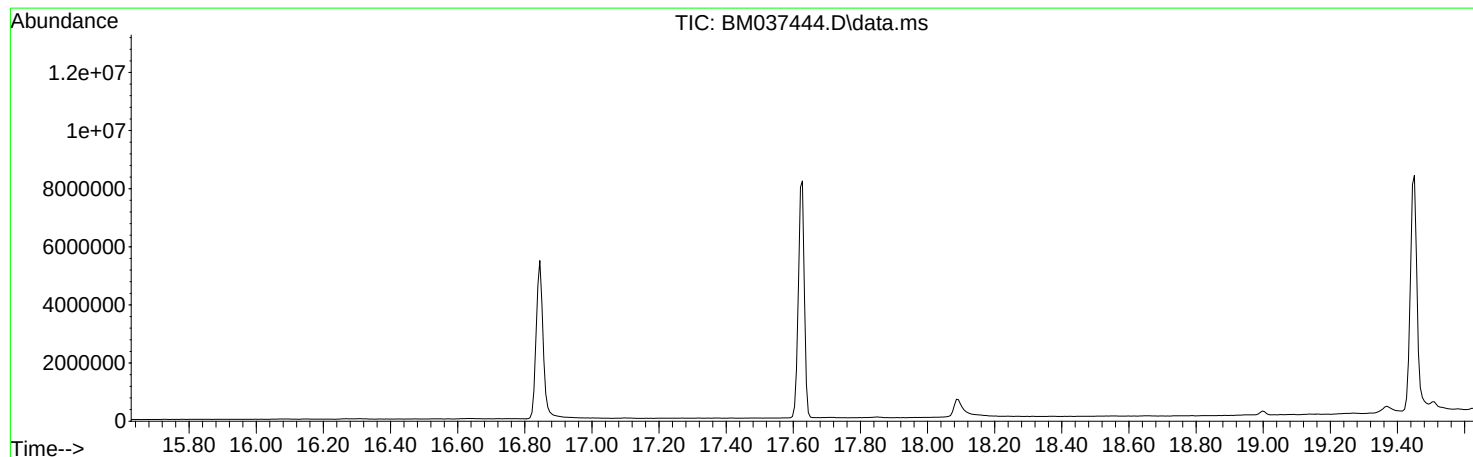




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	238996	PASS
68	69	0.00	2	1.5	3677	PASS
69	198	0.00	100	33.5	250989	PASS
70	69	0.00	2	0.6	1402	PASS
127	198	10	80	44.6	333594	PASS
197	198	0.00	2	0.4	2693	PASS
198	198	100	100	100.0	748437	PASS
199	198	5	9	6.7	50029	PASS
275	198	10	60	28.6	214379	PASS
365	198	1	100	3.7	27547	PASS
441	198	0.01	100	18.1	135331	PASS
442	442	50	100	100.0	901013	PASS
443	442	15	24	19.3	174101	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\  
Data File : BM037444.D  
Acq On    : 10 Nov 2022  10:32  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 10 15:57:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 02:08:14 2022
Response via : Initial Calibration

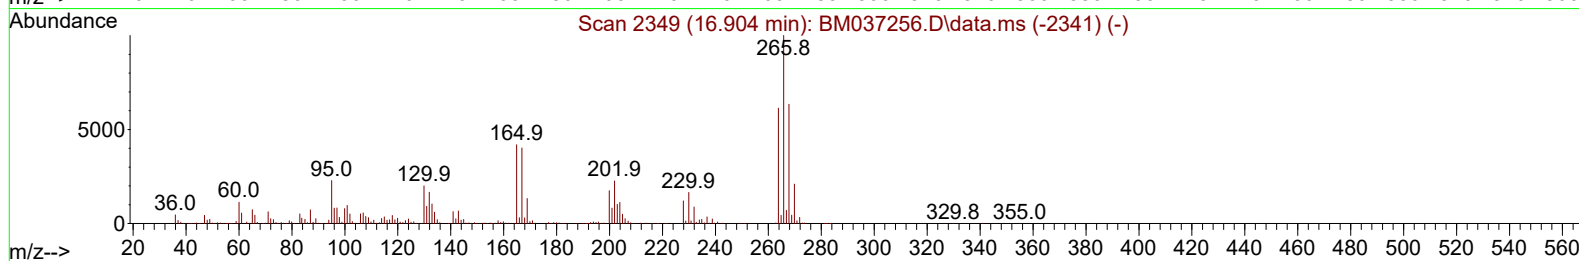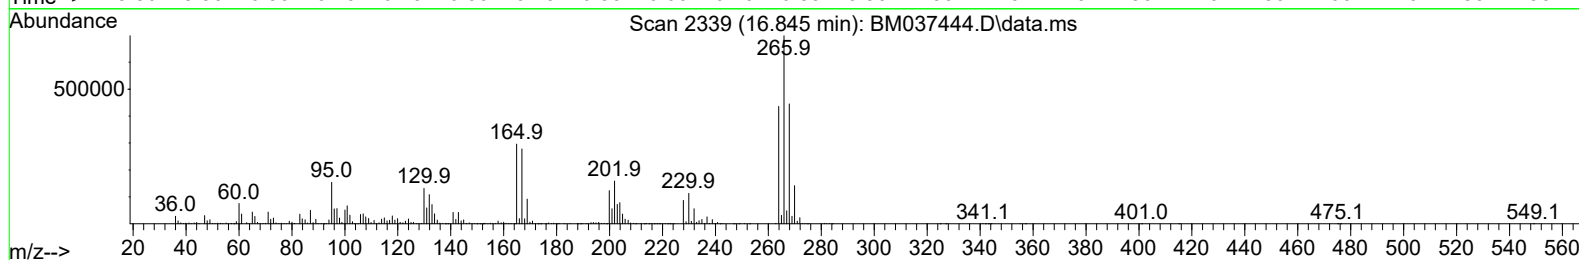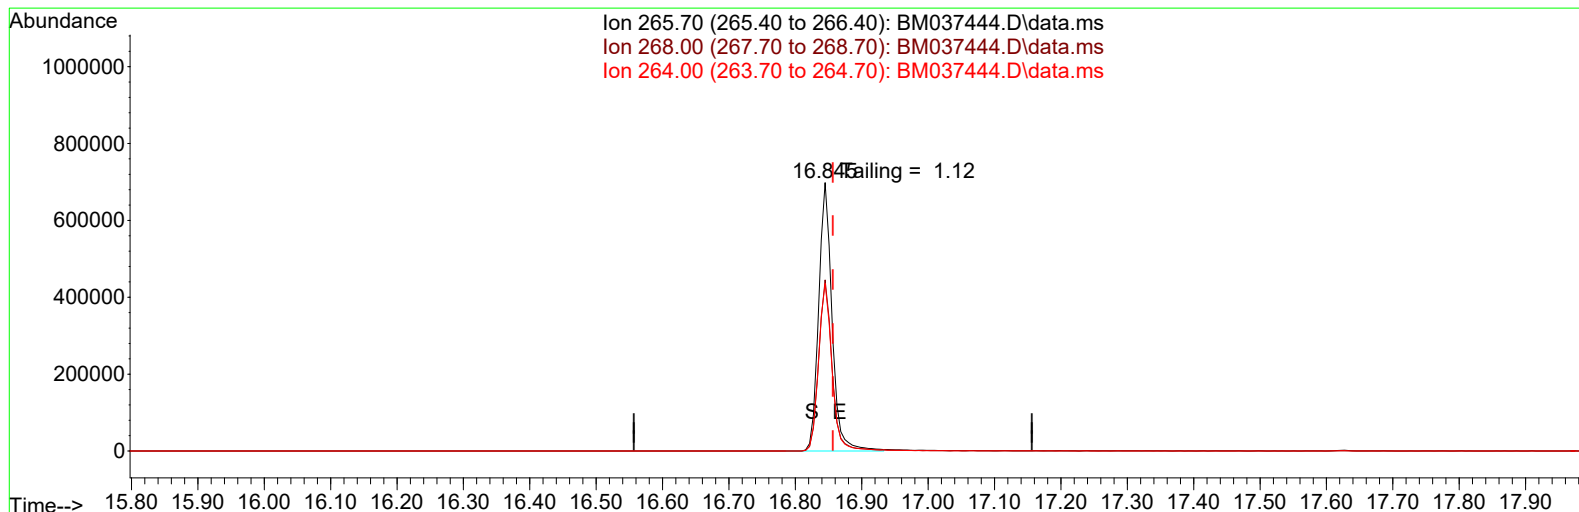

TIC: BM037444.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.012) 886032.28 ng




response **987250**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.72
264.00	61.40	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111022\
Data File : BM037444.D
Acq On : 10 Nov 2022 10:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 10 15:57:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 02:08:14 2022
Response via : Initial Calibration

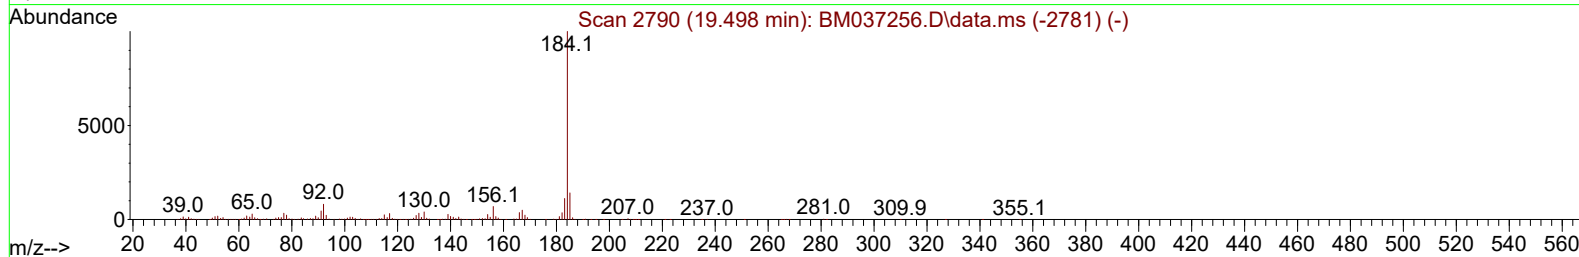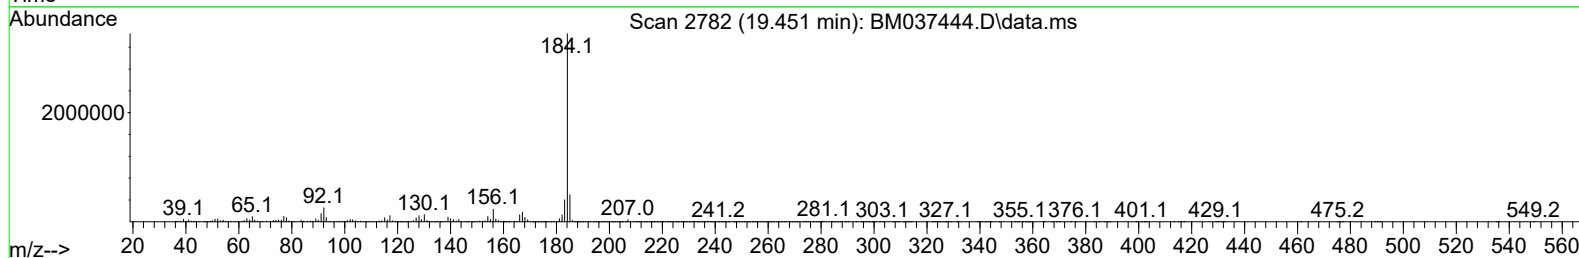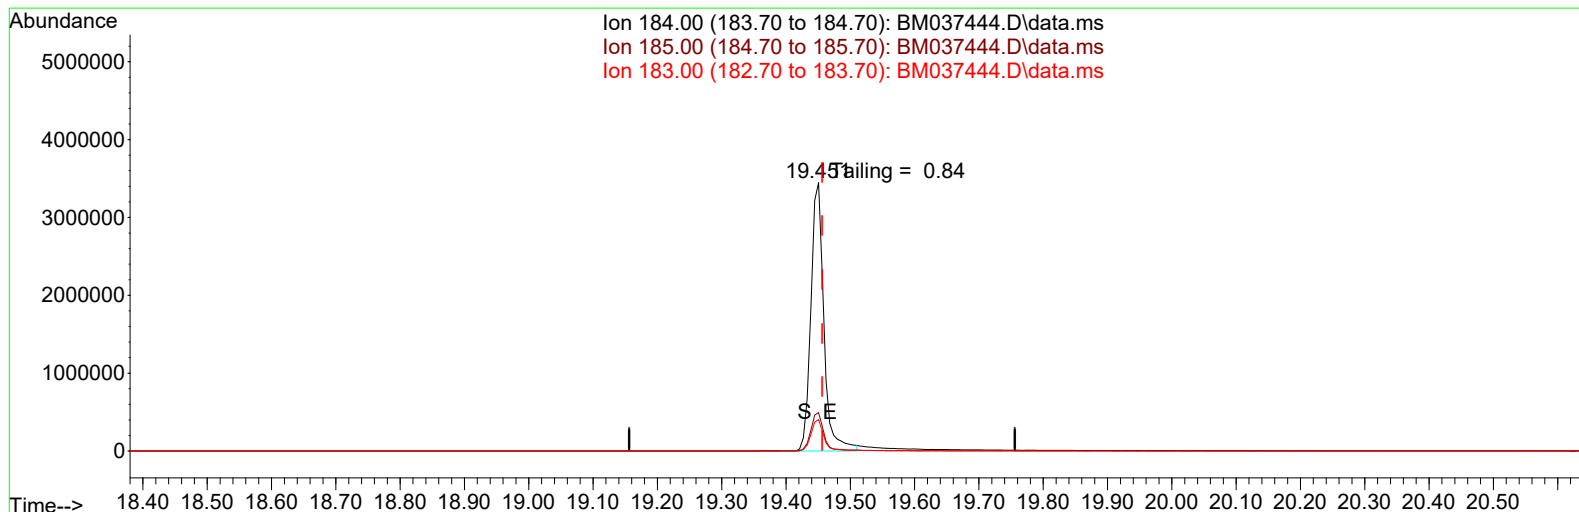

TIC: BM037444.D\data.ms

(77) Benzidine

19.451min (-0.006) 258618.52 ng

response 5113534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.34
183.00	11.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2022	BNA_M	<u>BM037444.D</u>
Compound Name	Response	Retention Time
DDT	2874364	20.668
DDD	48922	20.274
DDE	2183	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
51105	2925469	1.75

Instrument :
BNA_M
ClientSampleId :
DFTPP