

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111115\
 Data File : BM003106.D
 Acq On : 12 Nov 2015 05:01
 Operator : UM/IZ
 Sample : G4322-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4HT0

Quant Time: Nov 13 11:31:53 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 11:02:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	145991	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	683878	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.40	164	391478	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.14	188	778365	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	732596	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	724145	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.21	96	6248	2.02	ng/uL	0.00
5) Phenol-d5	6.91	99	134362	11.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	78286	11.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	117321	11.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	112196	12.06	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	57807	13.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	61301	14.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	114251	12.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	115389	9.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	369893	12.56	ng/ul	0.00
47) Acenaphthylene-d8	14.09	160	422148	11.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	49707	10.01	ng/ul	0.00
58) Fluorene-d10	15.39	176	282255	11.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	37428	10.38	ng/ul	0.00
71) Anthracene-d10	17.24	188	374898	10.86	ng/ul	0.00
79) Pyrene-d10	19.53	212	338040	9.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	279671	8.13	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.85	163	184309	6.14	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111115\
Data File : BM003106.D
Acq On : 12 Nov 2015 05:01
Operator : UM/IZ
Sample : G4322-19
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4HT0

Quant Time: Nov 13 11:31:53 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 11:02:42 2015
Response via : Initial Calibration

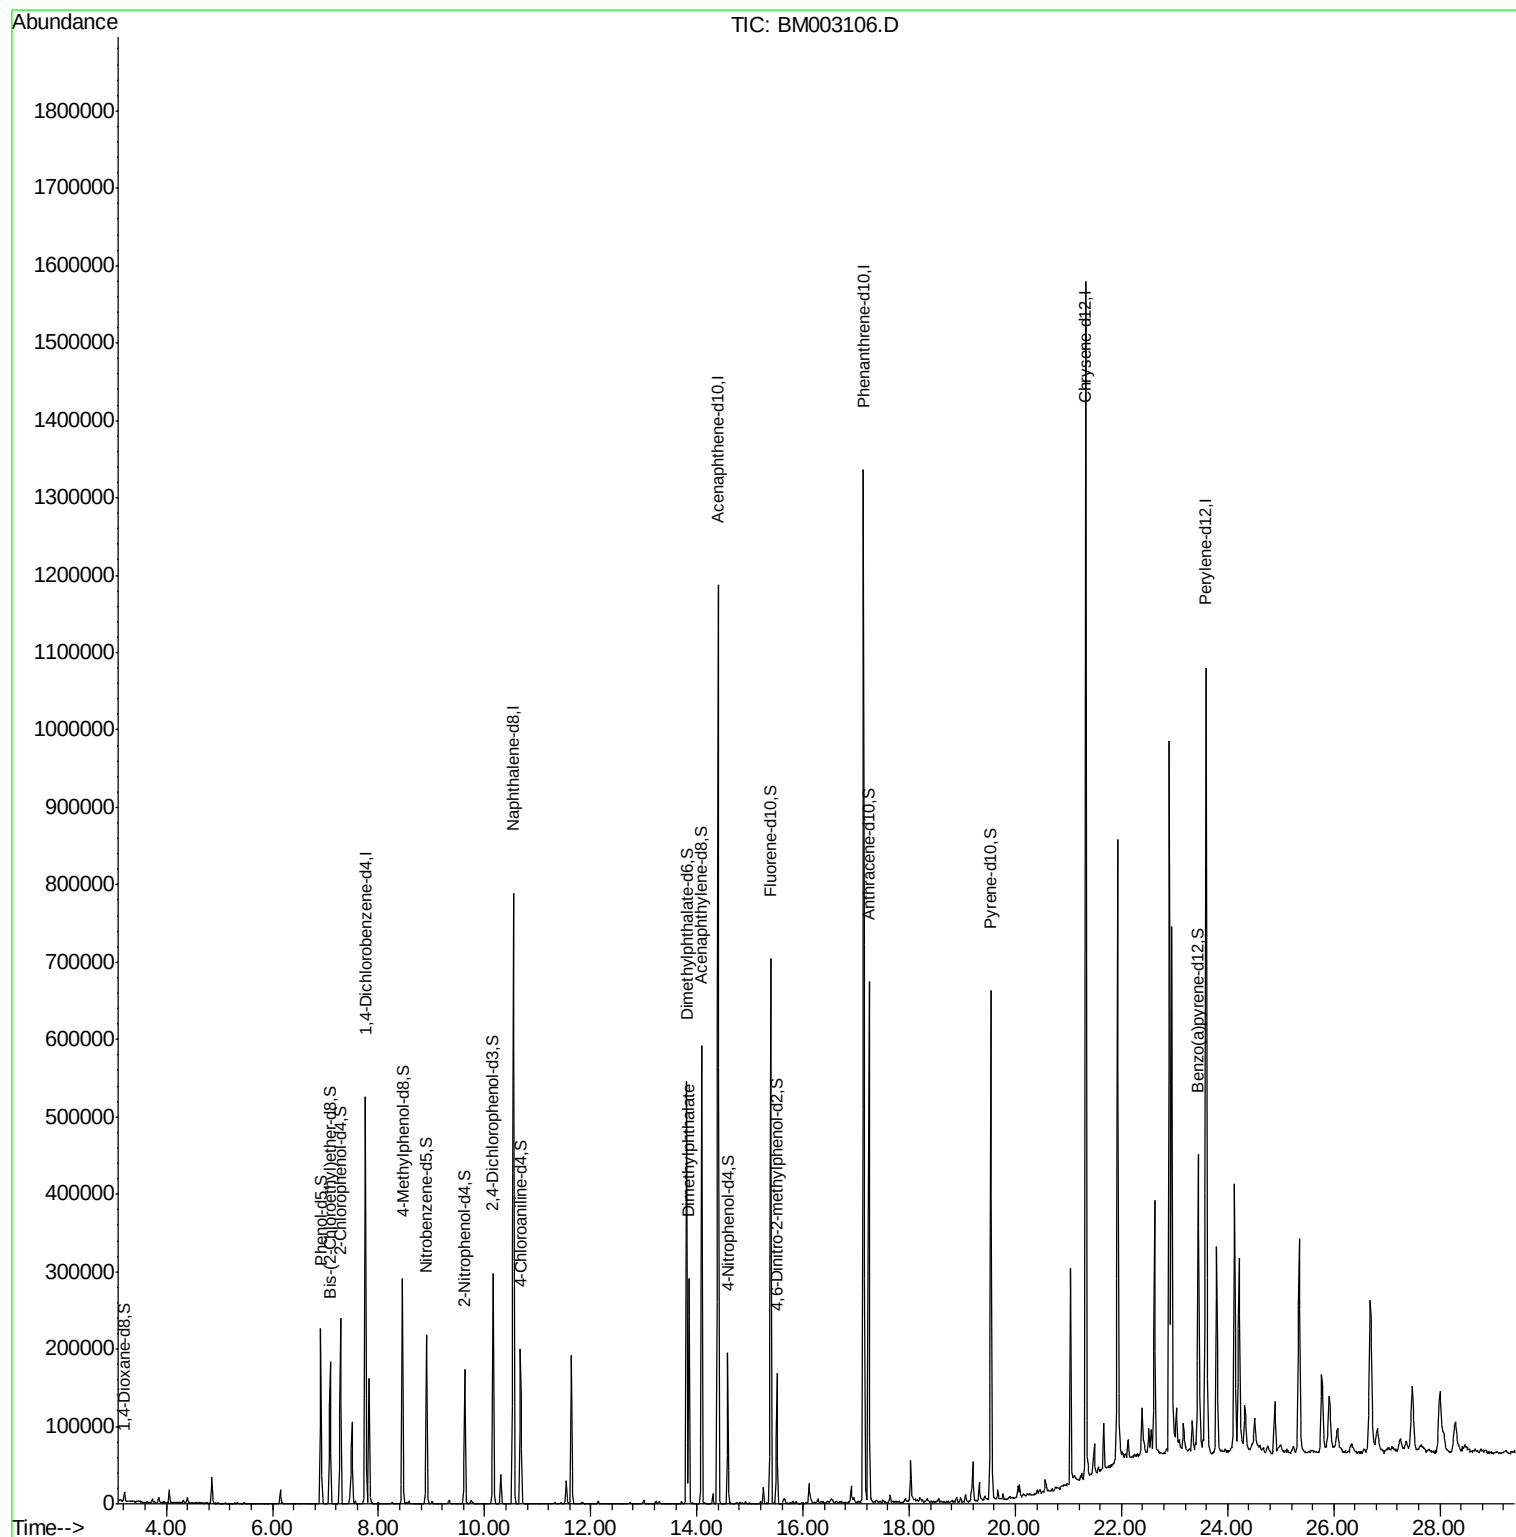

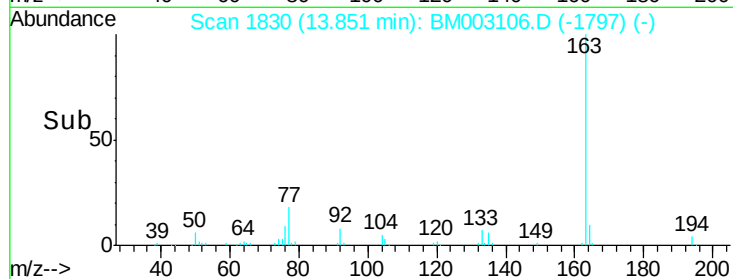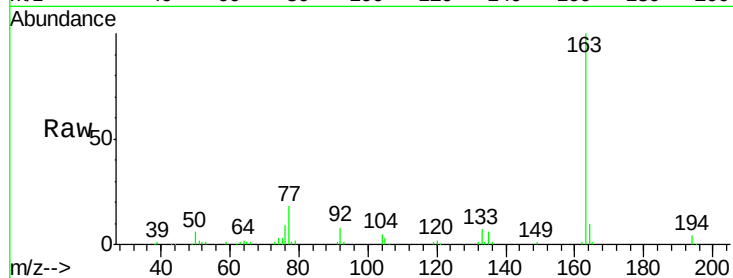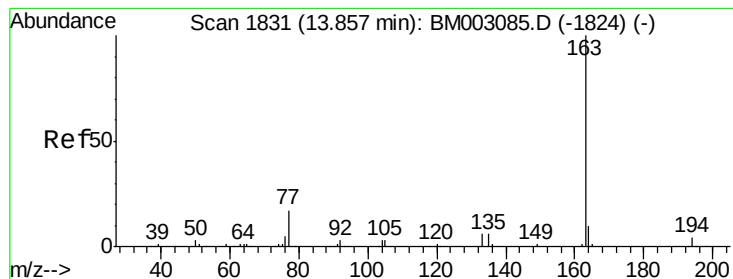

#45

Dimethylphthalate

Concen: 6.14 ng/ul

RT: 13.85 min Scan# 1830

Delta R.T. -0.01 min

Lab File: BM003106.D

Acq: 12 Nov 2015 05:01

Instrument :

BNA_M

ClientSampleId :

A4HT0

Tgt Ion:163 Resp: 184309

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.1 7.8 11.8

