

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
 Data File : BM003105.D
 Acq On : 12 Nov 2015 04:25
 Operator : UM/IZ
 Sample : G4322-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4HS9

Quant Time: Nov 13 11:31:45 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 13 11:02:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	132100	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	633262	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.40	164	389409	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.14	188	872106	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	830737	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	720510	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	5241	1.87	ng/uL	0.00
5) Phenol-d5	6.91	99	113402	10.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.08	67	71106	11.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.28	132	99762	11.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	98494	11.70	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	51534	13.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	54668	13.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.16	165	101119	11.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	113609	10.01	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	377176	12.87	ng/ul	0.00
47) Acenaphthylene-d8	14.09	160	425335	11.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	43686	8.85	ng/ul	0.00
58) Fluorene-d10	15.39	176	318882	12.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	42753	10.59	ng/ul	0.00
71) Anthracene-d10	17.24	188	471023	12.18	ng/ul	0.00
79) Pyrene-d10	19.54	212	491666	12.02	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	393512	11.49	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.85	163	177124	5.93	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
Data File : BM003105.D
Acq On : 12 Nov 2015 04:25
Operator : UM/IZ
Sample : G4322-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4HS9

Quant Time: Nov 13 11:31:45 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 13 11:02:42 2015
Response via : Initial Calibration

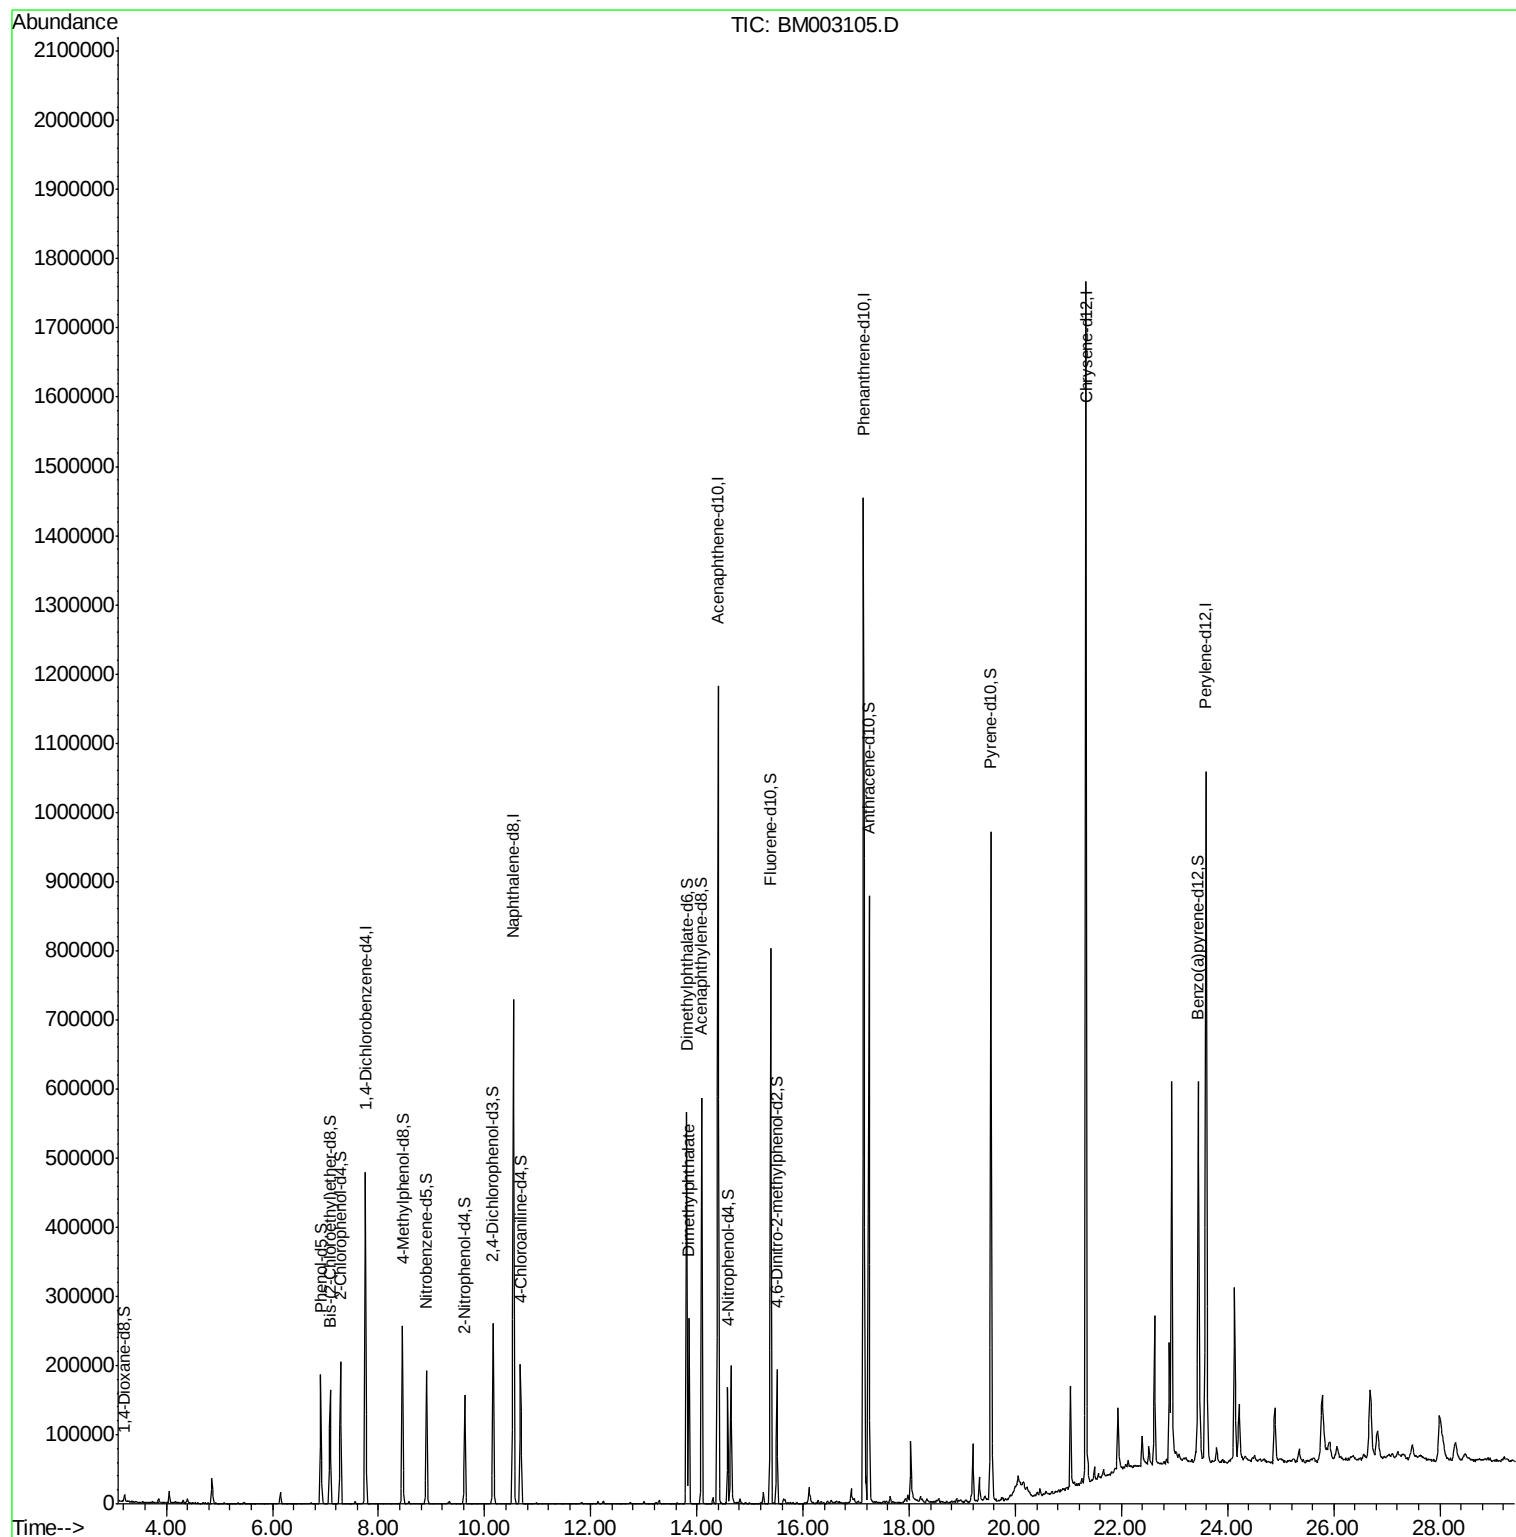

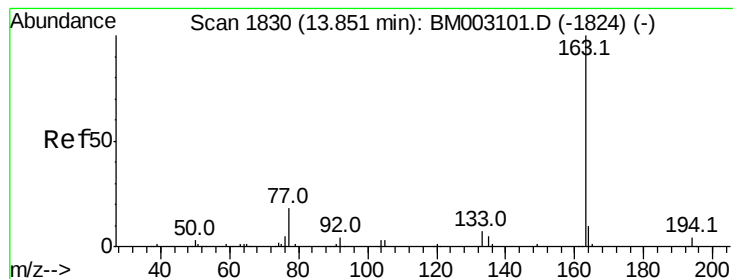

#45

Dimethylphthalate

Concen: 5.93 ng/ul

RT: 13.85 min Scan# 1830

Delta R.T. -0.01 min

Lab File: BM003105.D

Acq: 12 Nov 2015 04:25

Instrument :

BNA_M

ClientSampleId :

A4HS9


Tot Ion:163 Resp: 177124

Ion Ratio Lower Upper

163 100

194 3.6 3.2 4.8

164 10.6 7.8 11.8

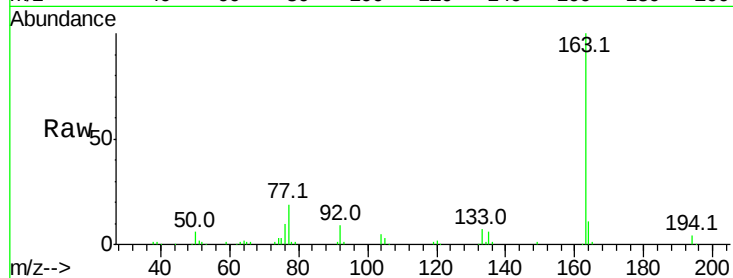

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

