

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
 Data File : BM003111.D
 Acq On : 12 Nov 2015 11:12
 Operator : UM/IZ
 Sample : G4374-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	29	rVB	6862	8235	0.30%	0.030%
2	3.551	76	79	83	rVB	8451	9551	0.35%	0.035%
3	3.851	126	130	134	rVB2	3117	4047	0.15%	0.015%
4	4.051	161	164	168	rVB3	8201	10136	0.37%	0.037%
5	4.310	204	208	214	rBV2	8979	10511	0.38%	0.038%
6	4.869	298	303	309	rVB2	6273	9616	0.35%	0.035%
7	5.293	371	375	381	rVB	5351	7423	0.27%	0.027%
8	5.798	458	461	465	rBV2	2851	3272	0.12%	0.012%
9	6.145	516	520	525	rVB	6144	8158	0.30%	0.030%
10	6.263	535	540	544	rVB	4394	5540	0.20%	0.020%
11	6.722	614	618	622	rVB2	3800	5403	0.20%	0.020%
12	6.910	643	650	657	rVB	110753	173361	6.28%	0.631%
13	7.081	673	679	691	rBB	349087	531679	19.26%	1.935%
14	7.281	706	713	721	rBB	384145	593463	21.50%	2.160%
15	7.751	786	793	800	rBV	486490	755857	27.38%	2.751%
16	7.810	800	803	808	rVB2	15164	21028	0.76%	0.077%
17	8.451	905	912	919	rBB	315356	495263	17.94%	1.803%
18	8.569	928	932	936	rBB	3492	5067	0.18%	0.018%
19	8.845	974	979	983	rBV	37105	56554	2.05%	0.206%
20	8.904	983	989	997	rVB	407547	658266	23.85%	2.396%
21	9.628	1105	1112	1119	rBB	341566	546098	19.78%	1.988%
22	9.745	1129	1132	1138	rBB	3530	5775	0.21%	0.021%
23	10.163	1196	1203	1212	rBB	519153	866957	31.41%	3.156%
24	10.451	1247	1252	1256	rBB2	9282	12960	0.47%	0.047%
25	10.545	1260	1268	1275	rBV	671576	1150654	41.68%	4.188%
26	10.598	1275	1277	1280	rVB2	3986	4197	0.15%	0.015%
27	10.680	1286	1291	1295	rBB	5008	7353	0.27%	0.027%
28	11.822	1480	1485	1490	rBB2	22097	31692	1.15%	0.115%
29	12.133	1534	1538	1544	rBB	7460	10949	0.40%	0.040%
30	12.316	1566	1569	1573	rBB	2734	3900	0.14%	0.014%
31	12.751	1638	1643	1646	rBB	5556	6470	0.23%	0.024%
32	12.998	1682	1685	1689	rBB	7808	10253	0.37%	0.037%
33	13.310	1732	1738	1745	rBB	91399	129835	4.70%	0.473%
34	13.810	1816	1823	1832	rBB	989857	1401649	50.77%	5.102%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
 Data File : BM003111.D
 Acq On : 12 Nov 2015 11:12
 Operator : UM/IZ
 Sample : G4374-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

35	14.092	1864	1871	1881	rBV	1119788	1665044	60.32%	6.060%
36	14.398	1916	1923	1931	rBB2	995837	1539811	55.78%	5.605%
37	14.480	1933	1937	1941	rBB	10982	13260	0.48%	0.048%
38	14.586	1949	1955	1961	rVB	98677	135039	4.89%	0.492%
39	14.810	1990	1993	1997	rBB	5634	5475	0.20%	0.020%
40	15.074	2033	2038	2043	rBB	18707	25189	0.91%	0.092%
41	15.204	2056	2060	2062	rBV2	4870	6133	0.22%	0.022%
42	15.392	2085	2092	2100	rBV	1514923	2130494	77.18%	7.755%
43	15.504	2106	2111	2118	rBV	392603	516588	18.71%	1.880%
44	15.633	2128	2133	2139	rVB	13484	17675	0.64%	0.064%
45	15.757	2150	2154	2158	rBV	6223	7643	0.28%	0.028%
46	16.927	2349	2353	2358	rVB	4606	5790	0.21%	0.021%
47	17.145	2383	2390	2396	rVB	1211083	1744301	63.19%	6.349%
48	17.239	2400	2406	2420	rVV2	1527815	2219958	80.42%	8.080%
49	17.433	2435	2439	2443	rBV	2632	3206	0.12%	0.012%
50	17.815	2499	2504	2509	rVB	125829	148367	5.37%	0.540%
51	18.033	2537	2541	2547	rBV	9196	11019	0.40%	0.040%
52	18.109	2550	2554	2556	rVV	4525	5392	0.20%	0.020%
53	18.139	2556	2559	2565	rVB	4775	6010	0.22%	0.022%
54	18.292	2581	2585	2589	rVB2	3124	3719	0.13%	0.014%
55	18.621	2638	2641	2644	rBV	3894	4312	0.16%	0.016%
56	19.174	2730	2735	2740	rVB	13812	18260	0.66%	0.066%
57	19.321	2757	2760	2764	rBV	5916	6398	0.23%	0.023%
58	19.427	2774	2778	2784	rBV	11670	17366	0.63%	0.063%
59	19.539	2791	2797	2807	rBV	1841910	2517583	91.20%	9.164%
60	20.150	2897	2901	2905	rBV4	2507	3687	0.13%	0.013%
61	20.468	2952	2955	2958	rBV2	4287	4232	0.15%	0.015%
62	21.339	3097	3103	3110	rBV	1702553	2123488	76.92%	7.729%
63	22.391	3279	3282	3286	rVB5	21938	29876	1.08%	0.109%
64	22.909	3367	3370	3375	rVB2	15895	24355	0.88%	0.089%
65	23.462	3456	3464	3477	rVB	1454592	2760545	100.00%	10.048%
66	23.603	3480	3488	3500	rVB	1140643	2149922	77.88%	7.825%
67	24.144	3576	3580	3587	rVB4	23395	42712	1.55%	0.155%


Sum of corrected areas: 27474021

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
Data File : BM003111.D
Acq On : 12 Nov 2015 11:12
Operator : UM/IZ
Sample : G4374-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

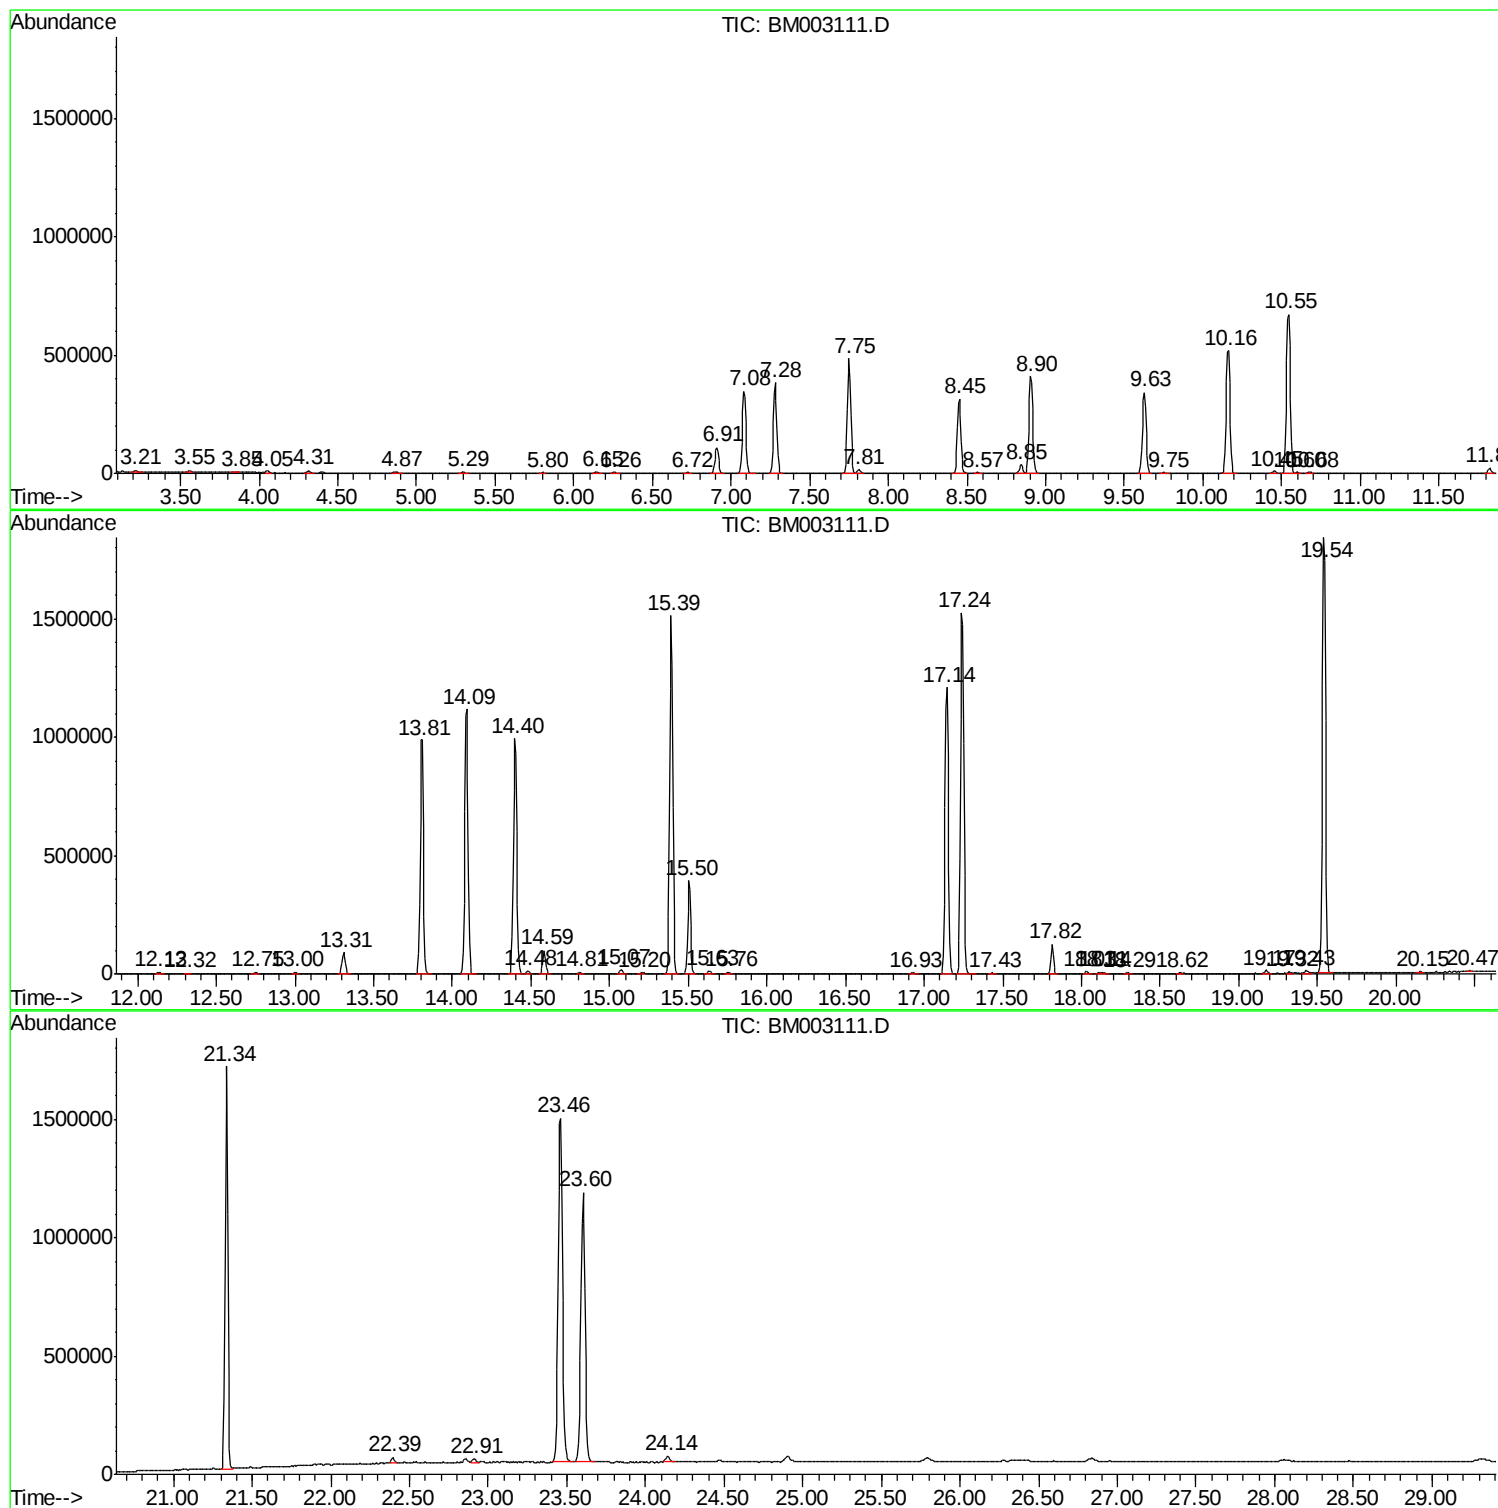

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111115\
Data File : BM003111.D
Acq On : 12 Nov 2015 11:12
Operator : UM/IZ
Sample : G4374-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111115\
Data File : BM003111.D
Acq On : 12 Nov 2015 11:12
Operator : UM/IZ
Sample : G4374-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc