

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
 Data File : BM003114.D
 Acq On : 12 Nov 2015 13:00
 Operator : UM/IZ
 Sample : G4374-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7F7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	30	rVB	5294	6909	0.25%	0.025%
2	4.058	162	165	168	rVB	5557	6259	0.23%	0.023%
3	4.393	217	222	227	rVB	2405	3546	0.13%	0.013%
4	4.869	297	303	306	rVB2	2179	3468	0.13%	0.012%
5	6.146	516	520	525	rBB	4581	6086	0.22%	0.022%
6	6.910	643	650	657	rBB	90216	136320	4.98%	0.490%
7	7.087	673	680	689	rBB	337041	529375	19.33%	1.903%
8	7.281	707	713	720	rBV	374503	565337	20.64%	2.032%
9	7.752	786	793	800	rBB	476511	734281	26.81%	2.640%
10	8.452	906	912	919	rBB	291251	450936	16.46%	1.621%
11	8.904	982	989	997	rBV	414122	665145	24.28%	2.391%
12	9.628	1105	1112	1119	rBB	350967	555179	20.27%	1.996%
13	10.157	1196	1202	1211	rBV	549020	892752	32.59%	3.209%
14	10.546	1260	1268	1279	rBB	699187	1173350	42.83%	4.218%
15	10.675	1287	1290	1295	rBB	3178	4277	0.16%	0.015%
16	12.134	1534	1538	1542	rBB2	8107	10805	0.39%	0.039%
17	13.804	1816	1822	1831	rBV	1134298	1551134	56.63%	5.576%
18	14.086	1863	1870	1878	rBV	1214324	1819785	66.43%	6.542%
19	14.398	1916	1923	1931	rVB2	1100511	1648248	60.17%	5.925%
20	14.581	1949	1954	1960	rBV	86917	120379	4.39%	0.433%
21	15.392	2085	2092	2101	rBB	1679424	2366387	86.39%	8.507%
22	15.504	2105	2111	2120	rVV	459279	596804	21.79%	2.145%
23	15.628	2127	2132	2140	rVB3	14789	18935	0.69%	0.068%
24	16.339	2248	2253	2258	rBV2	3078	4306	0.16%	0.015%
25	16.633	2297	2303	2307	rBV2	2278	2822	0.10%	0.010%
26	16.927	2349	2353	2357	rVB2	5447	6017	0.22%	0.022%
27	17.139	2383	2389	2395	rBV2	1357323	1957555	71.46%	7.037%
28	17.186	2395	2397	2400	rVV	9124	9469	0.35%	0.034%
29	17.239	2400	2406	2419	rVB2	1800783	2483566	90.67%	8.928%
30	17.510	2449	2452	2457	rVB3	5226	5531	0.20%	0.020%
31	18.027	2537	2540	2549	rBV	35632	47404	1.73%	0.170%
32	18.104	2549	2553	2557	rVB3	2100	2966	0.11%	0.011%
33	18.745	2659	2662	2669	rVB2	3907	4371	0.16%	0.016%
34	19.168	2730	2734	2741	rBV	15393	21412	0.78%	0.077%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
Data File : BM003114.D
Acq On : 12 Nov 2015 13:00
Operator : UM/IZ
Sample : G4374-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Title : SVOA CALIBRATION

35	19.316	2755	2759	2769	rBV	43909	52762	1.93%	0.190%
36	19.421	2773	2777	2784	rBV	12840	19276	0.70%	0.069%
37	19.539	2791	2797	2808	rVB	2019164	2739260	100.00%	9.847%
38	20.092	2887	2891	2894	rBV3	1900	3441	0.13%	0.012%
39	20.145	2896	2900	2901	rBV3	3491	4625	0.17%	0.017%
40	21.045	3050	3053	3057	rBV2	5903	8071	0.29%	0.029%
41	21.251	3086	3088	3090	rVB2	4554	3362	0.12%	0.012%
42	21.333	3096	3102	3110	rBV	1582444	2006988	73.27%	7.215%
43	21.927	3199	3203	3207	rBV	41134	52353	1.91%	0.188%
44	22.392	3279	3282	3286	rVB	25092	28116	1.03%	0.101%
45	22.904	3365	3369	3374	rBV	75733	102430	3.74%	0.368%
46	23.451	3455	3462	3475	rVV	1181327	2332028	85.13%	8.383%
47	23.598	3479	3487	3500	rVB	953219	1833612	66.94%	6.592%
48	24.133	3574	3578	3587	rVB	58148	114519	4.18%	0.412%
49	24.898	3703	3708	3723	rVB2	48139	104968	3.83%	0.377%


Sum of corrected areas: 27816927

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111115\
Data File : BM003114.D
Acq On : 12 Nov 2015 13:00
Operator : UM/IZ
Sample : G4374-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

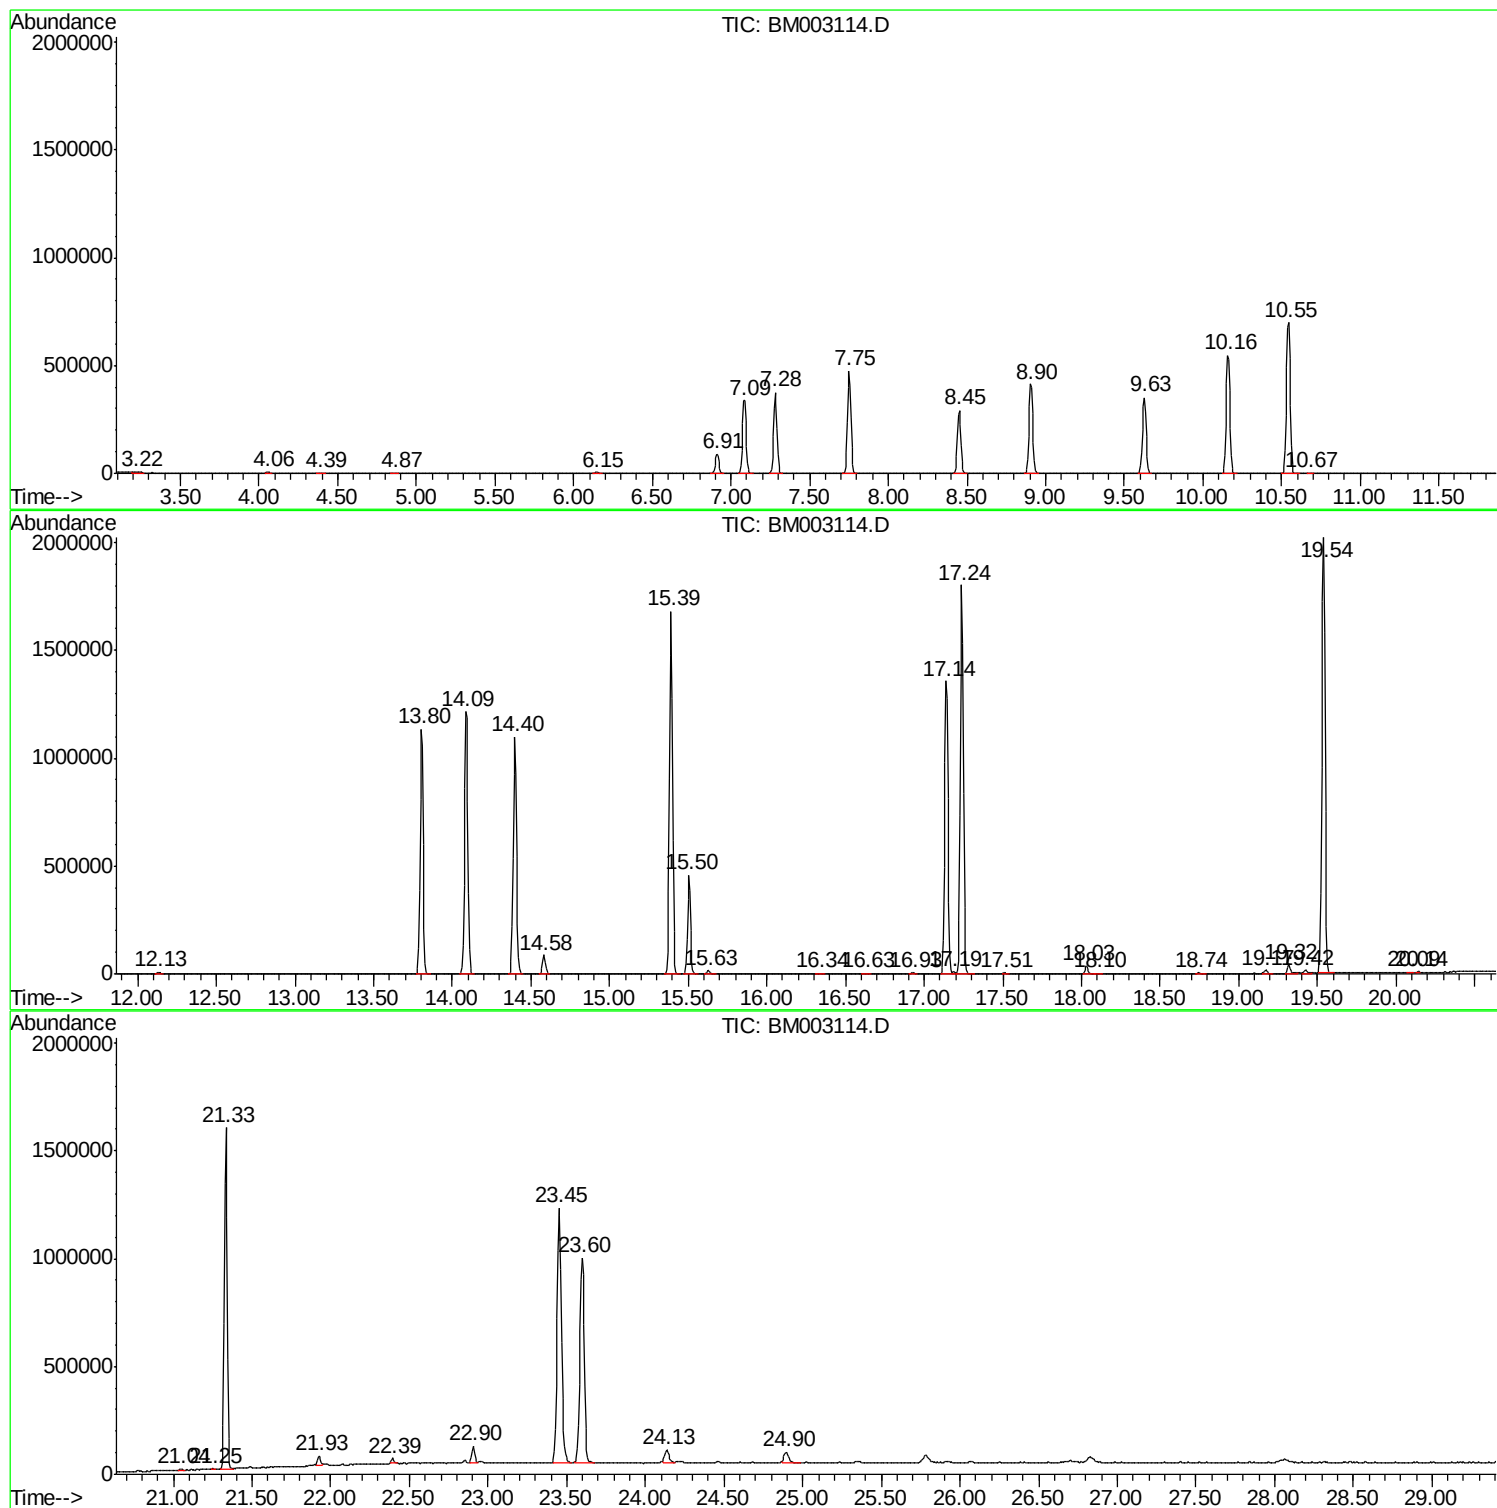

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111115\
Data File : BM003114.D
Acq On : 12 Nov 2015 13:00
Operator : UM/IZ
Sample : G4374-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111115\
Data File : BM003114.D
Acq On : 12 Nov 2015 13:00
Operator : UM/IZ
Sample : G4374-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7F7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc