


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111120\
Data File : BM027789.D
Acq On : 11 Nov 2020 13:49
Operator : JU/CG
Sample : L4661-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F4R04

Manual Integrations
APPROVED

Sohil
11/12/2020 8:19:58 AM

Quant Time: Nov 11 14:37:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 11 11:32:20 2020
Response via : Initial Calibration

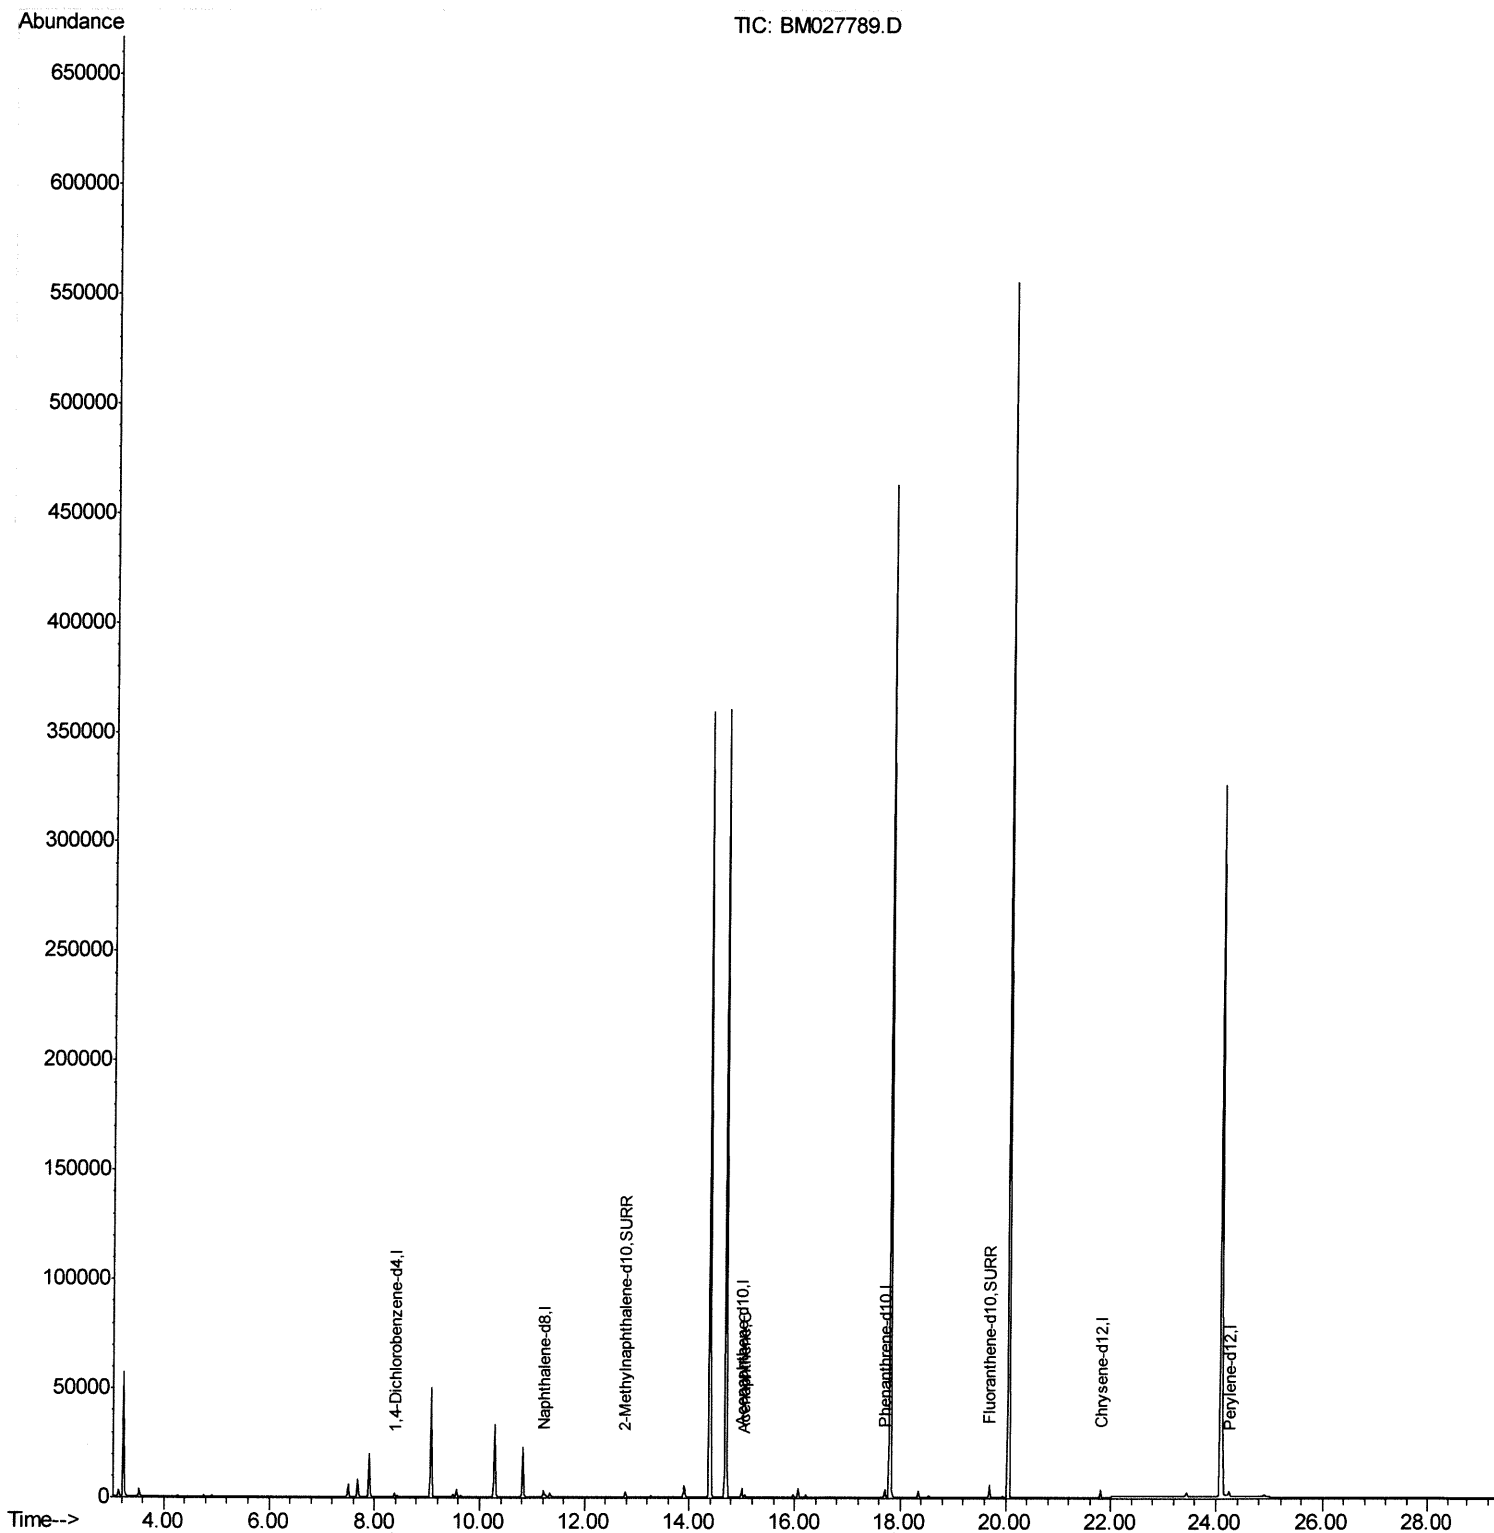




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111120\
 Data File : BM027789.D
 Acq On : 11 Nov 2020 13:49
 Operator : JU/CG
 Sample : L4661-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R04

Manual Integrations
 APPROVED

Sohil
 11/12/2020 8:19:58 AM

Quant Time: Nov 11 14:36:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 11:32:20 2020
 Response via : Initial Calibration

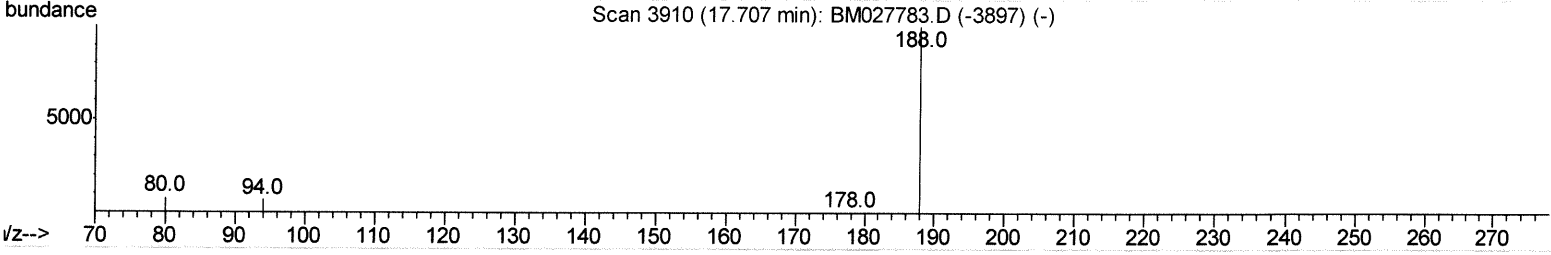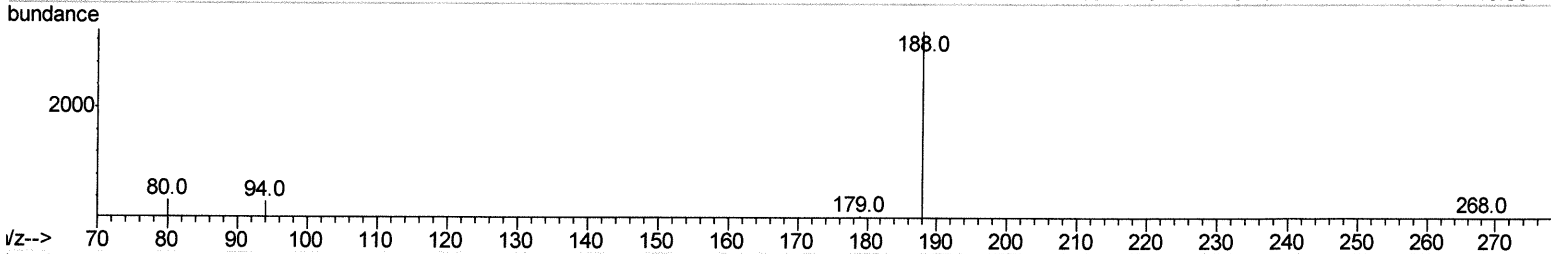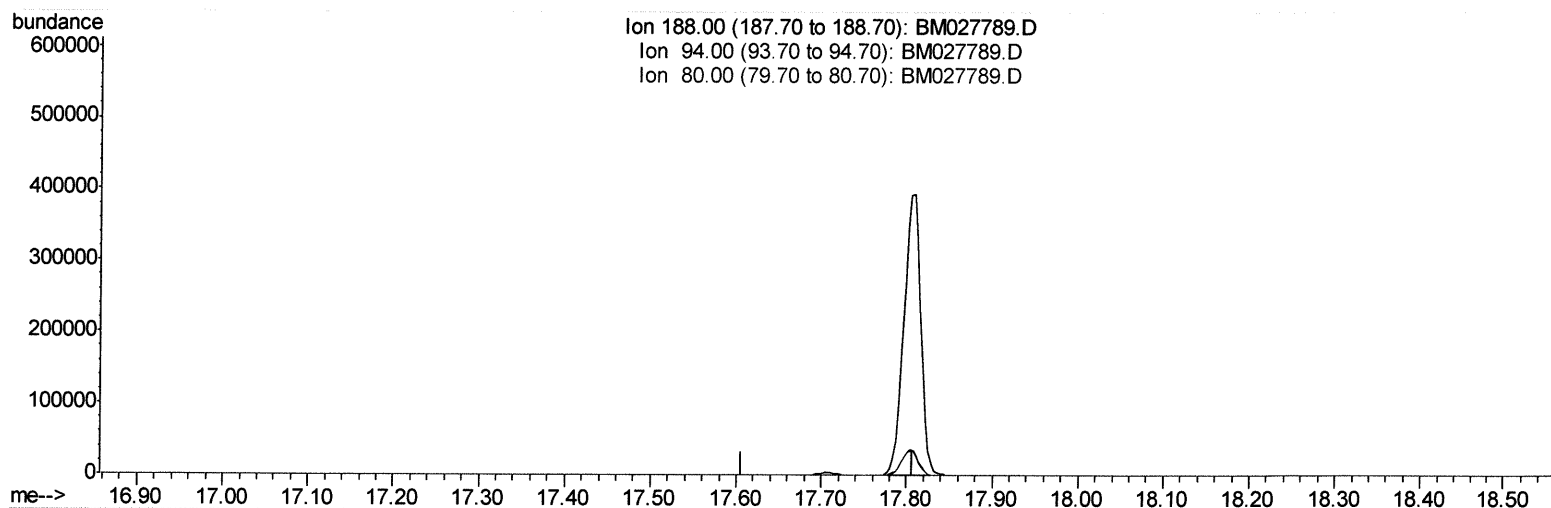

TIC: BM027789.D

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.50	0.00#
80.00	9.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111120\
 Data File : BM027789.D
 Acq On : 11 Nov 2020 13:49
 Operator : JU/CG
 Sample : L4661-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R04

Manual Integrations
 APPROVED

Sohil
 11/12/2020 8:19:58 AM

Quant Time: Nov 11 14:36:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 11:32:20 2020
 Response via : Initial Calibration

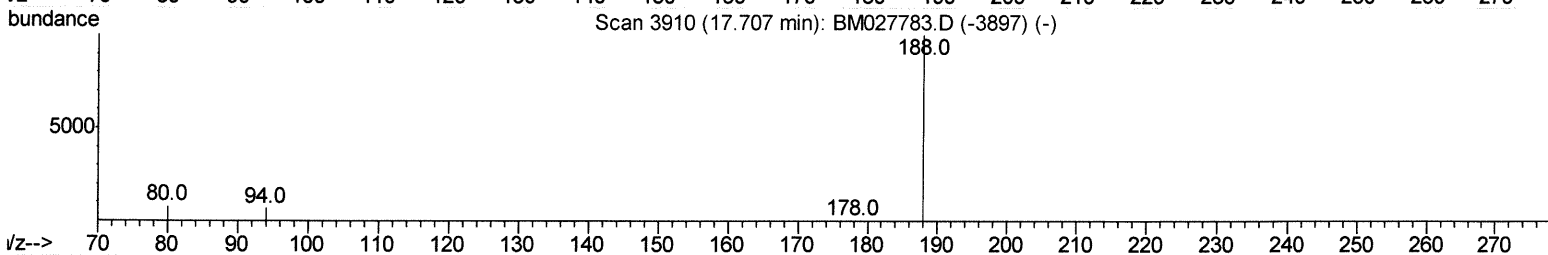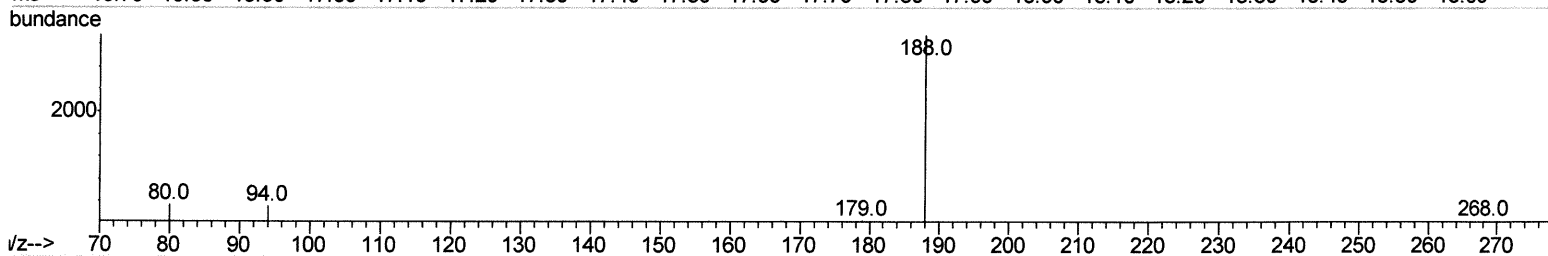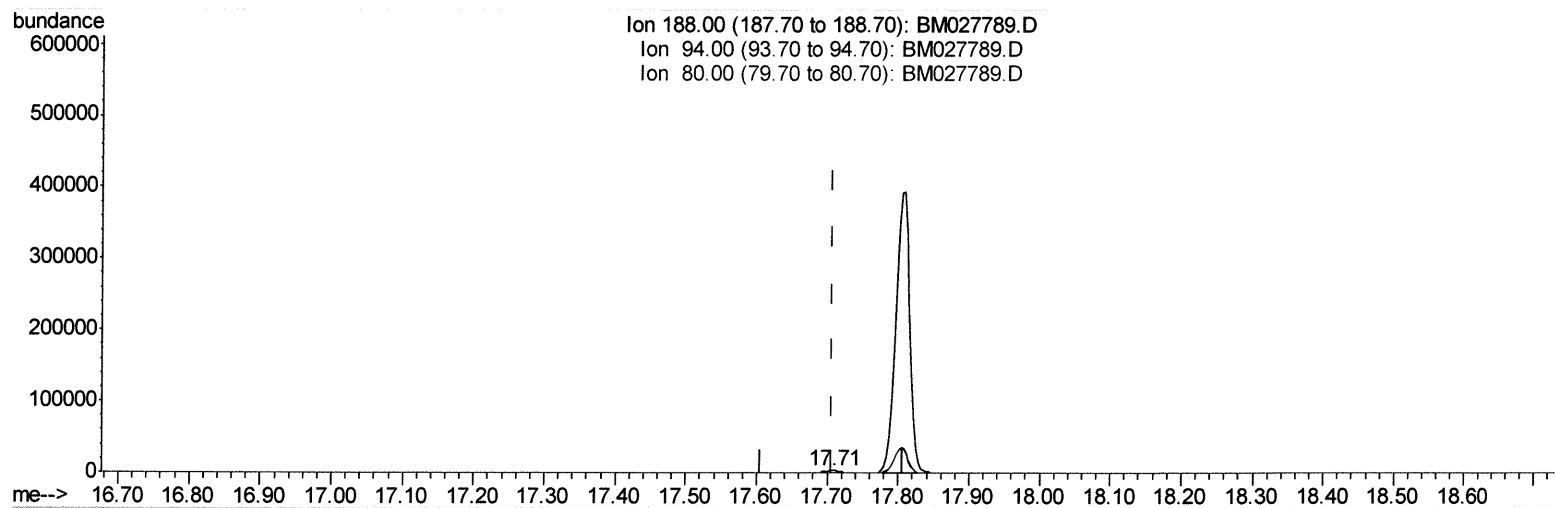

TIC: BM027789.D

(10) Phenanthrene-d10 (I)

17.707min (-0.000) 0.40ng/ul m

response 4677

Ion	Exp%	Act%
188.00	100	100
94.00	8.50	9.26
80.00	9.60	10.06
0.00	0.00	0.00

JU 11/12/20

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111120\
 Data File : BM027789.D
 Acq On : 11 Nov 2020 13:49
 Operator : JU/CG
 Sample : L4661-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F4R04

Manual Integrations
 APPROVED

Sohil
 11/12/2020 8:19:58 AM

Quant Time: Nov 11 14:37:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM111020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 11 11:32:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	942	0.40	ng/ul	0.00
2) Naphthalene-d8	11.22	136	3706	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.99	164	2431	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	4677m	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	3741	0.40	ng/ul	0.00
20) Perylene-d12	24.25	264	3139	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.78	152	2620	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6110	0.44	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Acenaphthene	15.05	153	1166	0.127	ng/ul#	26

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 11/12/20