
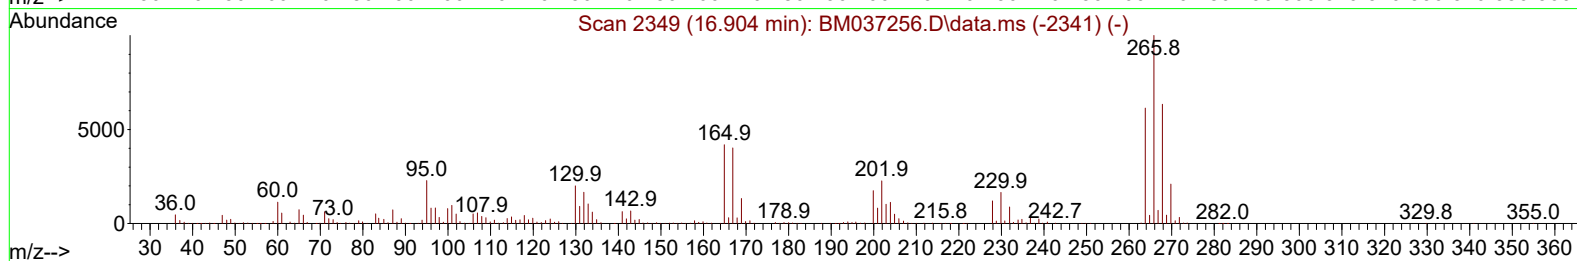
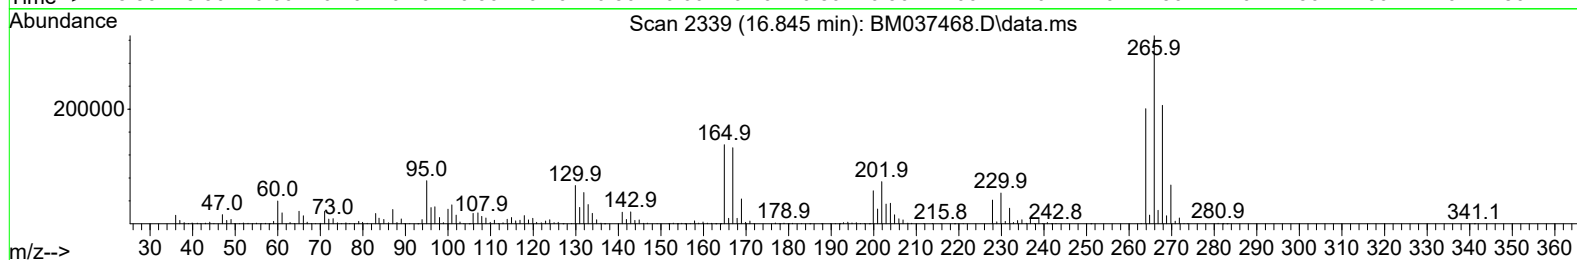


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111122\
Data File : BM037468.D
Acq On : 11 Nov 2022 15:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:05:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:49:50 2022
Response via : Initial Calibration

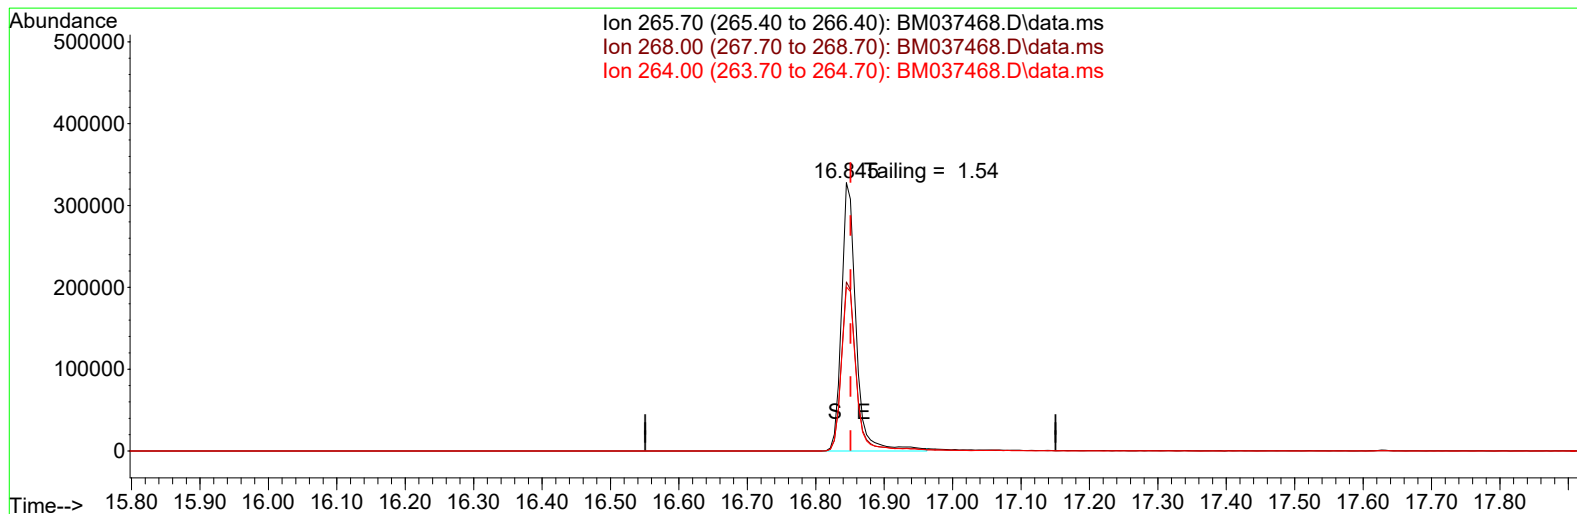

TIC: BM037468.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.006) 155923.50 ng

response 475617

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.04
264.00	61.40	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111122\
Data File : BM037468.D
Acq On : 11 Nov 2022 15:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:05:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:49:50 2022
Response via : Initial Calibration

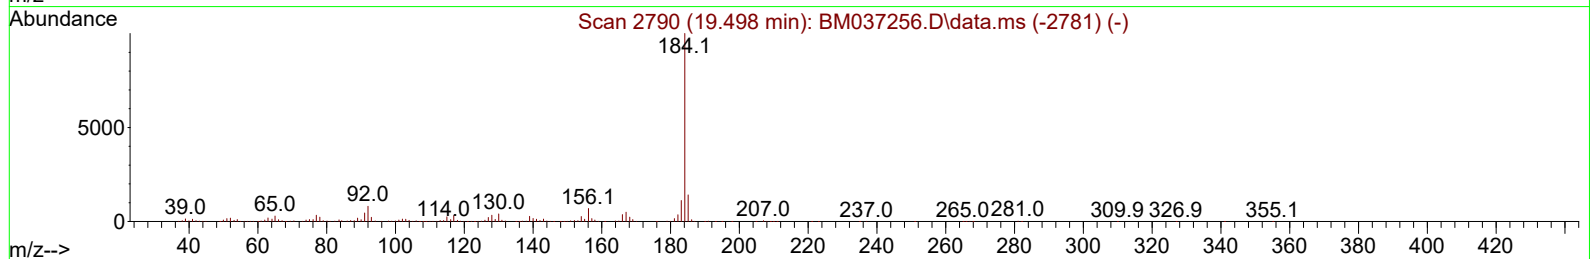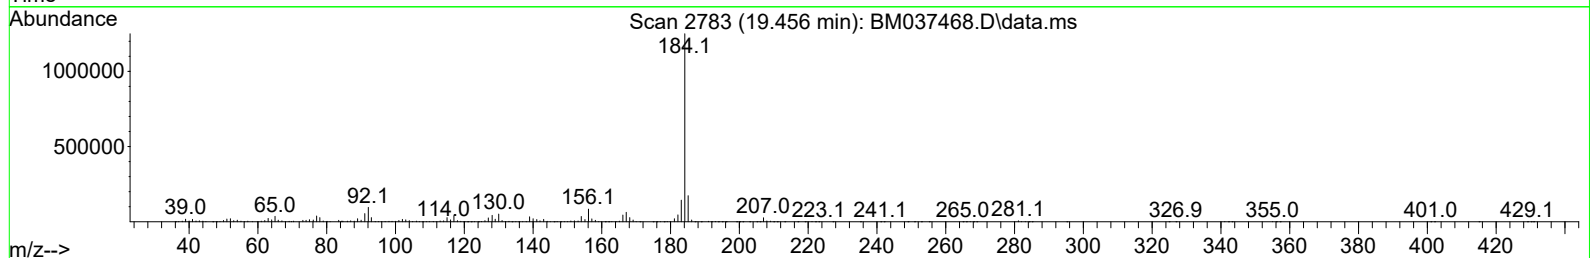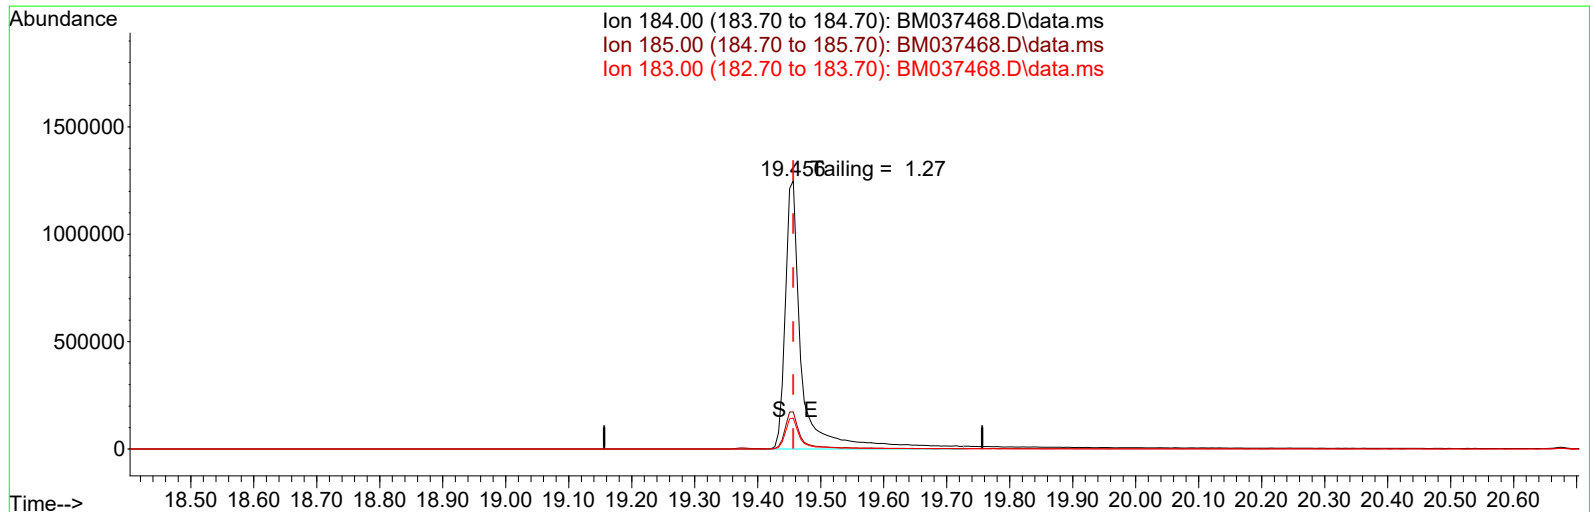

TIC: BM037468.D\data.ms

(77) Benzidine**19.456min (0.000) 73978.81 ng****response 2292297**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.85
183.00	11.20	11.54
0.00	0.00	0.00