
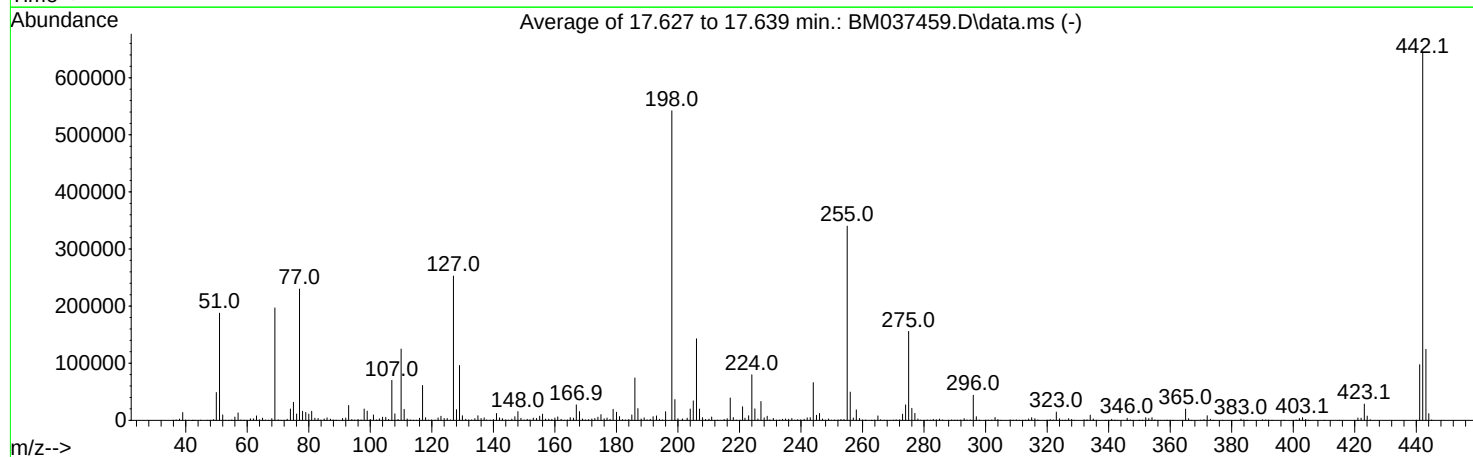


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111122\
Data File : BM037459.D
Acq On : 11 Nov 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 11 22:49:50 2022

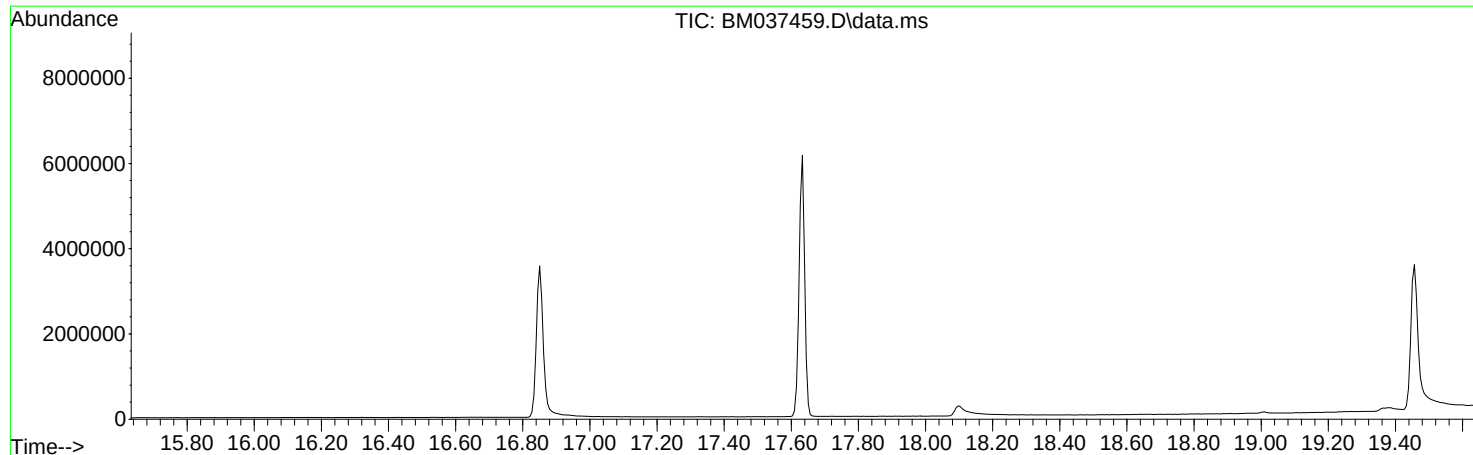




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	187565	PASS
68	69	0.00	2	1.4	2851	PASS
69	198	0.00	100	36.3	196777	PASS
70	69	0.00	2	0.5	964	PASS
127	198	10	80	46.6	252693	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	542016	PASS
199	198	5	9	6.7	36413	PASS
275	198	10	60	28.7	155659	PASS
365	198	1	100	3.7	19859	PASS
441	198	0.01	100	18.0	97344	PASS
442	442	50	100	100.0	644309	PASS
443	442	15	24	19.3	124333	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111122\
Data File : BM037459.D
Acq On : 11 Nov 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 12 05:04:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:49:50 2022
Response via : Initial Calibration

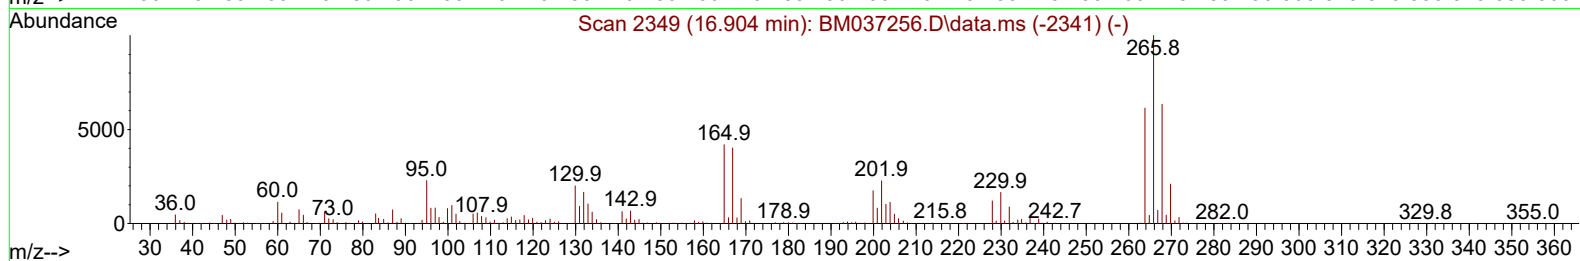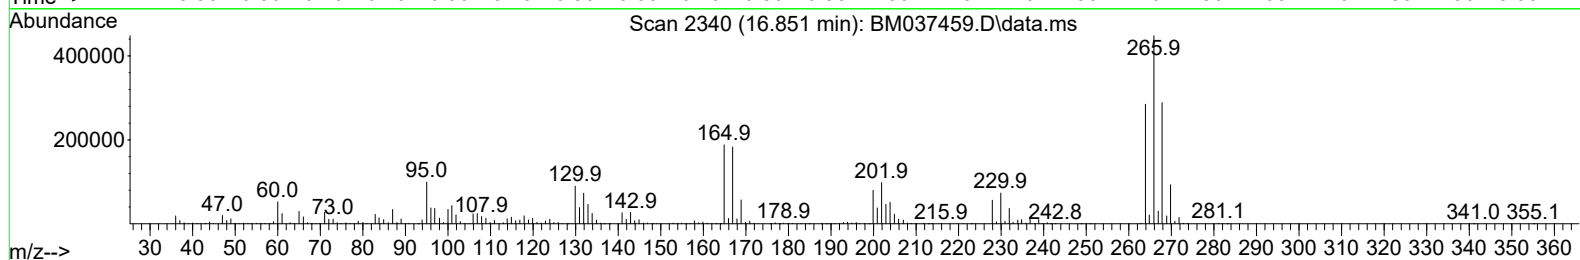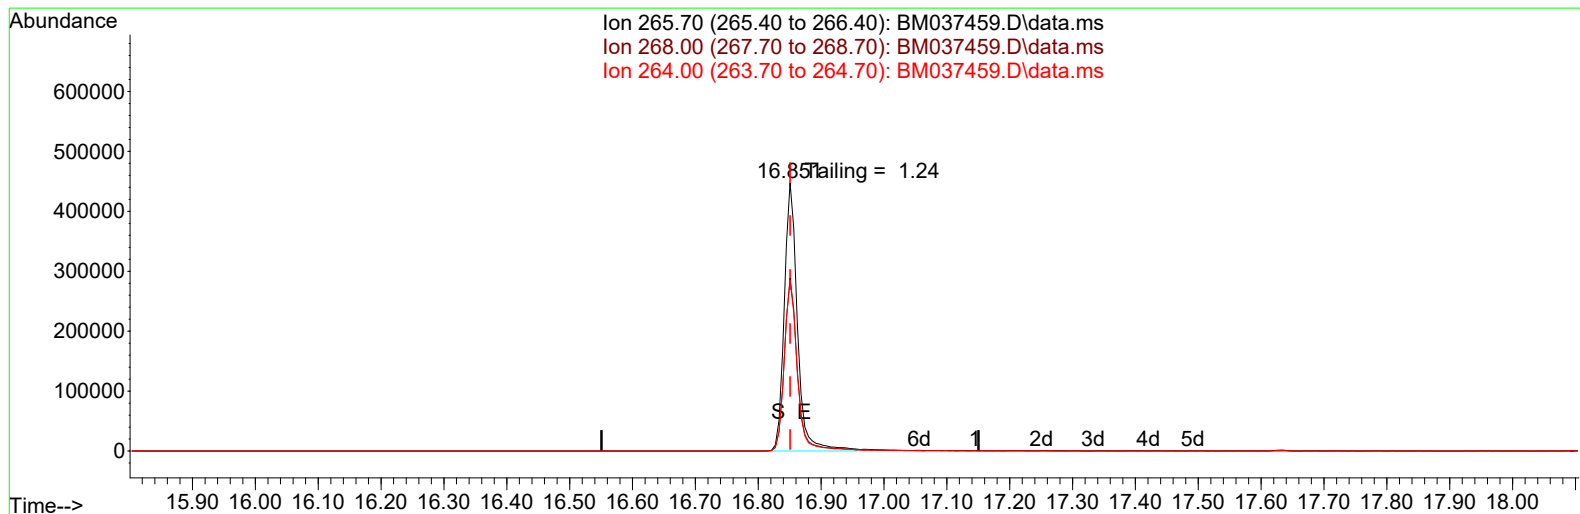

TIC: BM037459.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.000) 25006.56 ng m




response 669508

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	64.45
264.00	61.40	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111122\
Data File : BM037459.D
Acq On : 11 Nov 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 12 05:04:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:49:50 2022
Response via : Initial Calibration

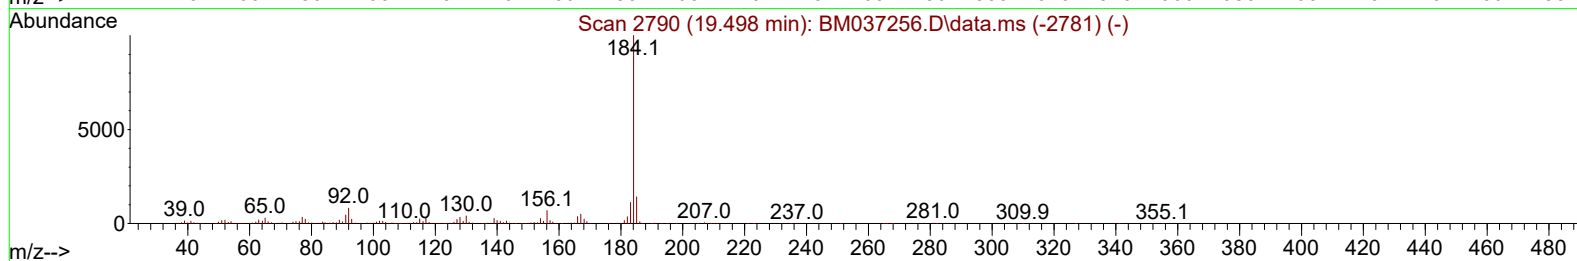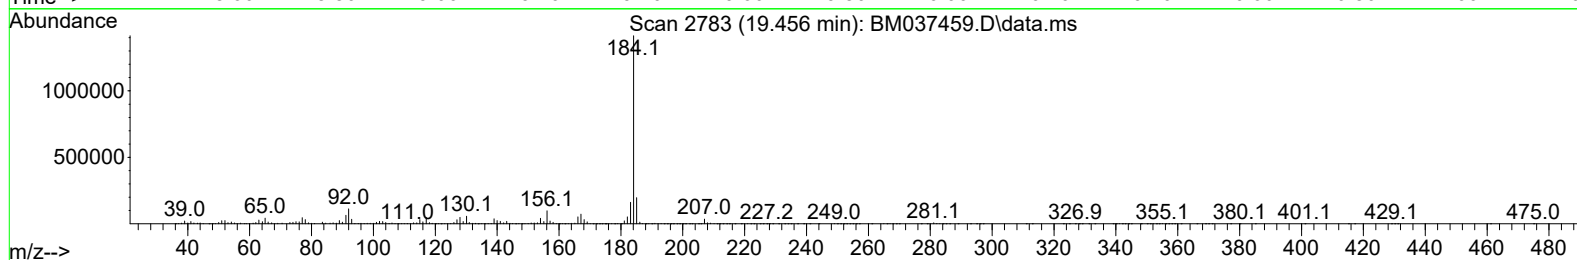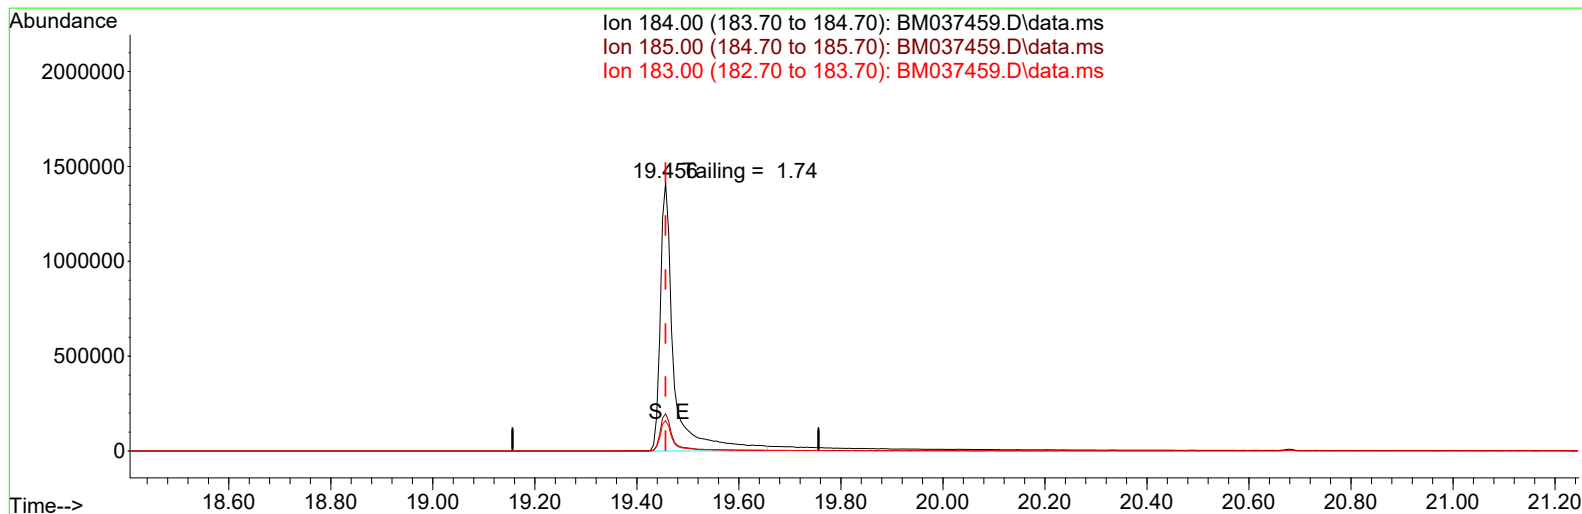

TIC: BM037459.D\data.ms

(77) Benzidine

19.456min (-0.000) 726208.32 ng m

response 3042885

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.92
183.00	11.20	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_M	<u>BM037459.D</u>
Compound Name	Response	Retention Time
DDT	1795830	20.68
DDD	32950	20.244
DDE	1569	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34519	1830349	1.89

Instrument :
BNA_M
ClientSampleId :
DFTPP