

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048580.D
 Acq On : 11 Nov 2024 11:32
 Operator : RC/JU
 Sample : P4686-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCP54

Quant Time: Nov 18 23:36:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 07 22:50:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	140767	20.000	ng/ul	0.00
20) Naphthalene-d8	10.445	136	569938	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	345189	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	707619	20.000	ng/ul	0.00
79) Chrysene-d12	21.286	240	634130	20.000	ng/ul	0.00
88) Perylene-d12	24.192	264	777033	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	11611	3.288	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.840	99	221357	20.657	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.998	67	128123	19.906	ng/ul	0.00
11) 2-Chlorophenol-d4	7.193	132	187059	21.074	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	169284	20.091	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128	91661	22.189	ng/ul	0.00
24) 2-Nitrophenol-d4	9.540	143	97512	22.193	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.075	165	199019	24.382	ng/ul	0.00
31) 4-Chloroaniline-d4	10.598	131	212855	18.359	ng/ul	0.00
46) Dimethylphthalate-d6	13.727	166	732720	33.252	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	784323	30.190	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	135211	33.037	ng/ul	0.00
60) Fluorene-d10	15.304	176	645629	33.566	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	93704	26.323	ng/ul	0.00
73) Anthracene-d10	17.157	188	1023781	34.189	ng/ul	0.00
81) Pyrene-d10	19.451	212	1238847	38.928	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.991	264	1285971	35.421	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.716	266	1049299	204.984	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048580.D
Acq On : 11 Nov 2024 11:32
Operator : RC/JU
Sample : P4686-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCP54

Quant Time: Nov 18 23:36:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 07 22:50:20 2024
Response via : Initial Calibration

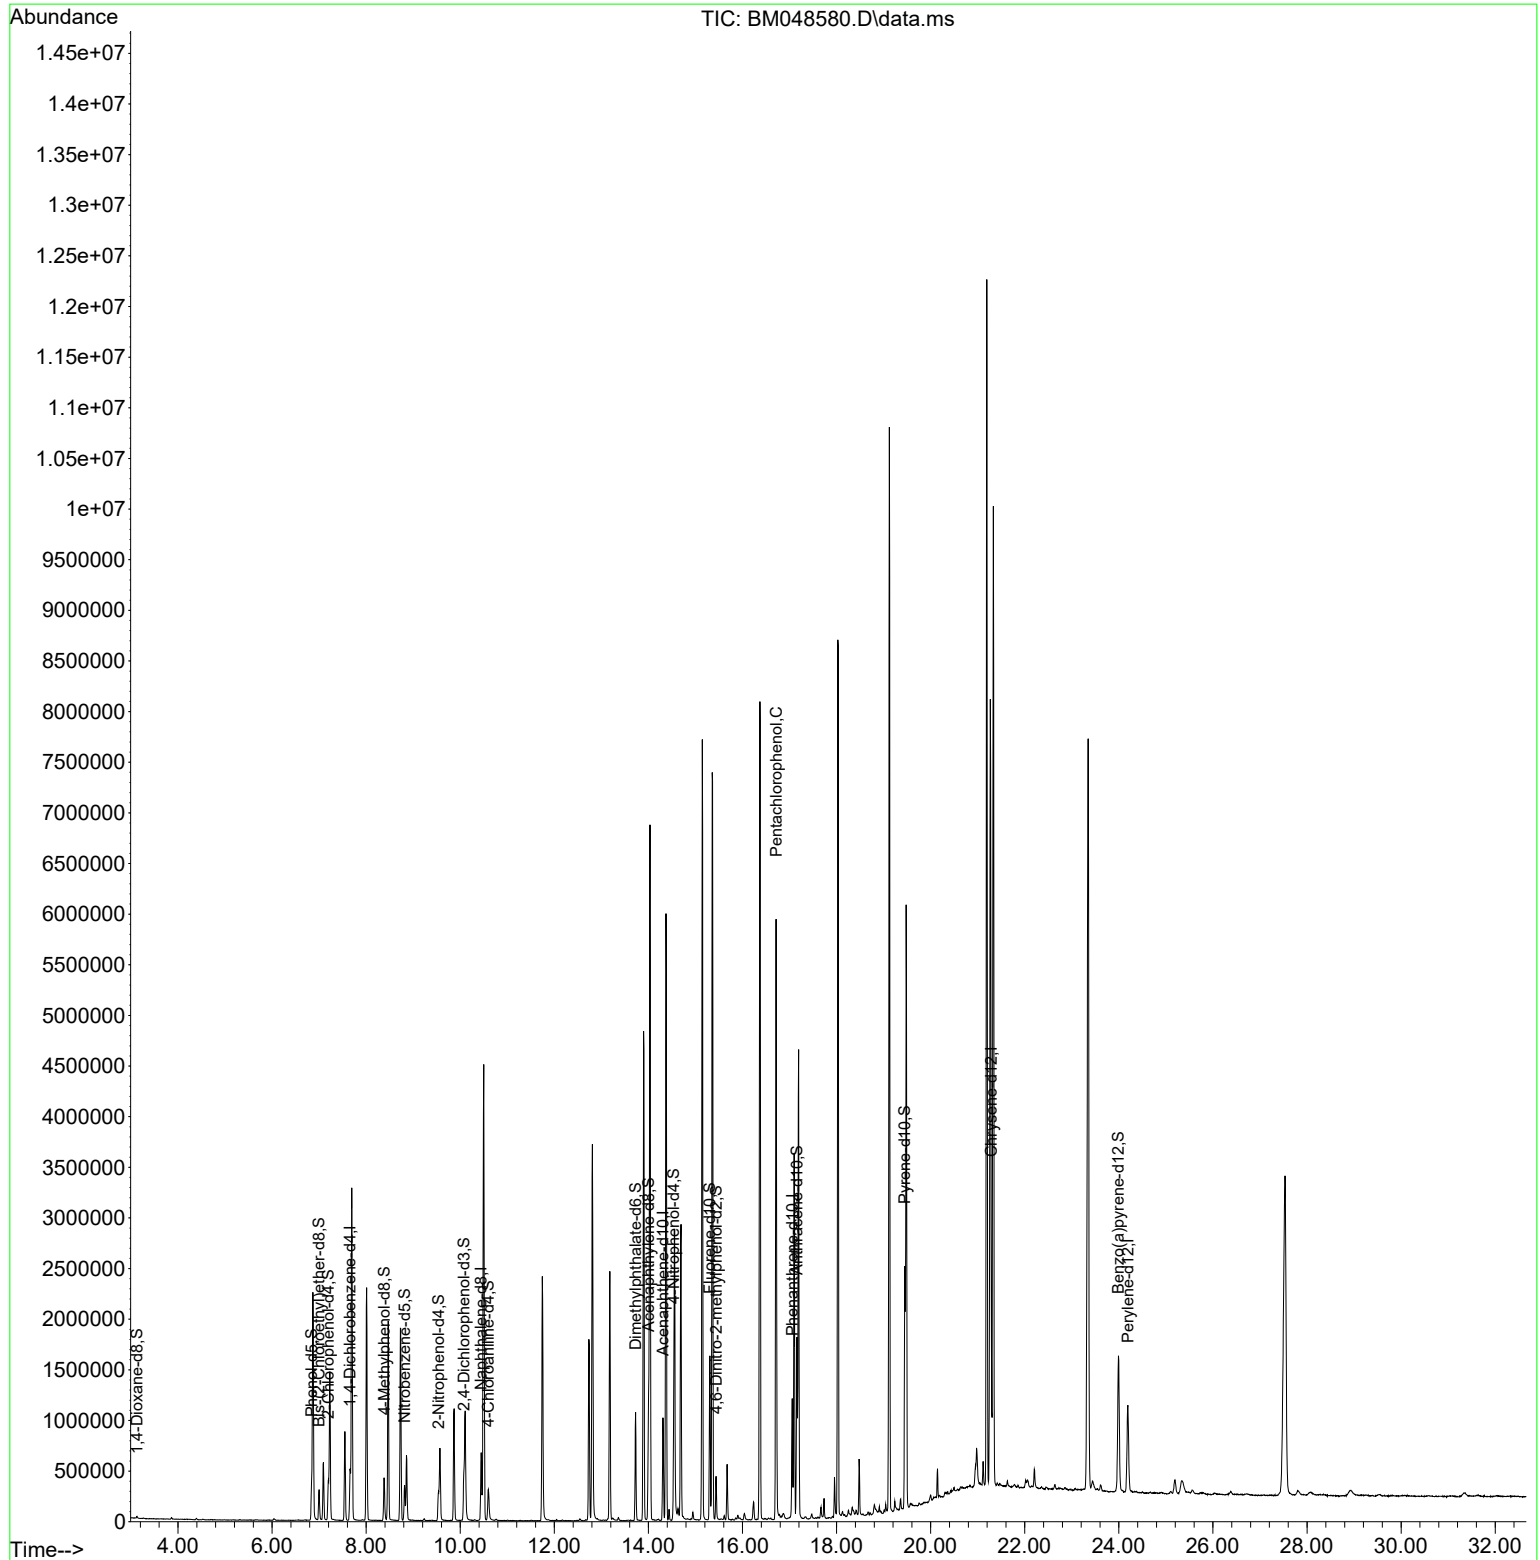

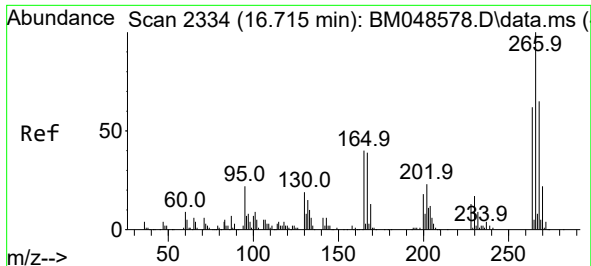

#71

Pentachlorophenol

Concen: 204.984 ng/ul

RT: 16.716 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM048580.D


Acq: 11 Nov 2024 11:32

Instrument :

BNA_M

ClientSampleId :

GCP54

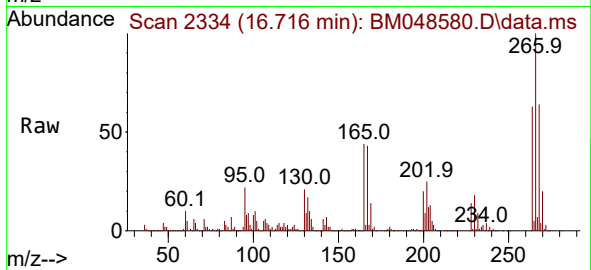

Tgt Ion:266 Resp: 1049299

Ion Ratio Lower Upper

266 100

264 63.2 51.1 76.7

268 64.3 53.2 79.8

