

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048581.D
 Acq On : 11 Nov 2024 12:15
 Operator : RC/JU
 Sample : P4686-05DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCP54DL

Quant Time: Nov 18 23:40:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 07 22:50:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	136567	20.000	ng/ul	0.00
20) Naphthalene-d8	10.445	136	558193	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	337664	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.056	188	688301	20.000	ng/ul	0.00
79) Chrysene-d12	21.280	240	681358	20.000	ng/ul	0.00
88) Perylene-d12	24.191	264	794113	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.128	96	2533	0.739	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.845	99	41531	3.995	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.998	67	24383	3.905	ng/ul	0.00
11) 2-Chlorophenol-d4	7.198	132	35204	4.088	ng/ul	0.00
15) 4-Methylphenol-d8	8.386	113	28813	3.525	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	16018	3.959	ng/ul	0.00
24) 2-Nitrophenol-d4	9.539	143	15926	3.701	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.086	165	36391	4.552	ng/ul	0.00
31) 4-Chloroaniline-d4	10.616	131	34165	3.009	ng/ul	0.02
46) Dimethylphthalate-d6	13.727	166	140619	6.524	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	149520	5.884	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	18460	4.611	ng/ul	0.00
60) Fluorene-d10	15.304	176	127137	6.757	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	12017	3.471	ng/ul	0.00
73) Anthracene-d10	17.156	188	202656	6.958	ng/ul	0.00
81) Pyrene-d10	19.450	212	249894	7.308	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.991	264	259265	6.988	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.715	266	208156	41.805	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048581.D
Acq On : 11 Nov 2024 12:15
Operator : RC/JU
Sample : P4686-05DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCP54DL


Quant Time: Nov 18 23:40:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 07 22:50:20 2024
Response via : Initial Calibration

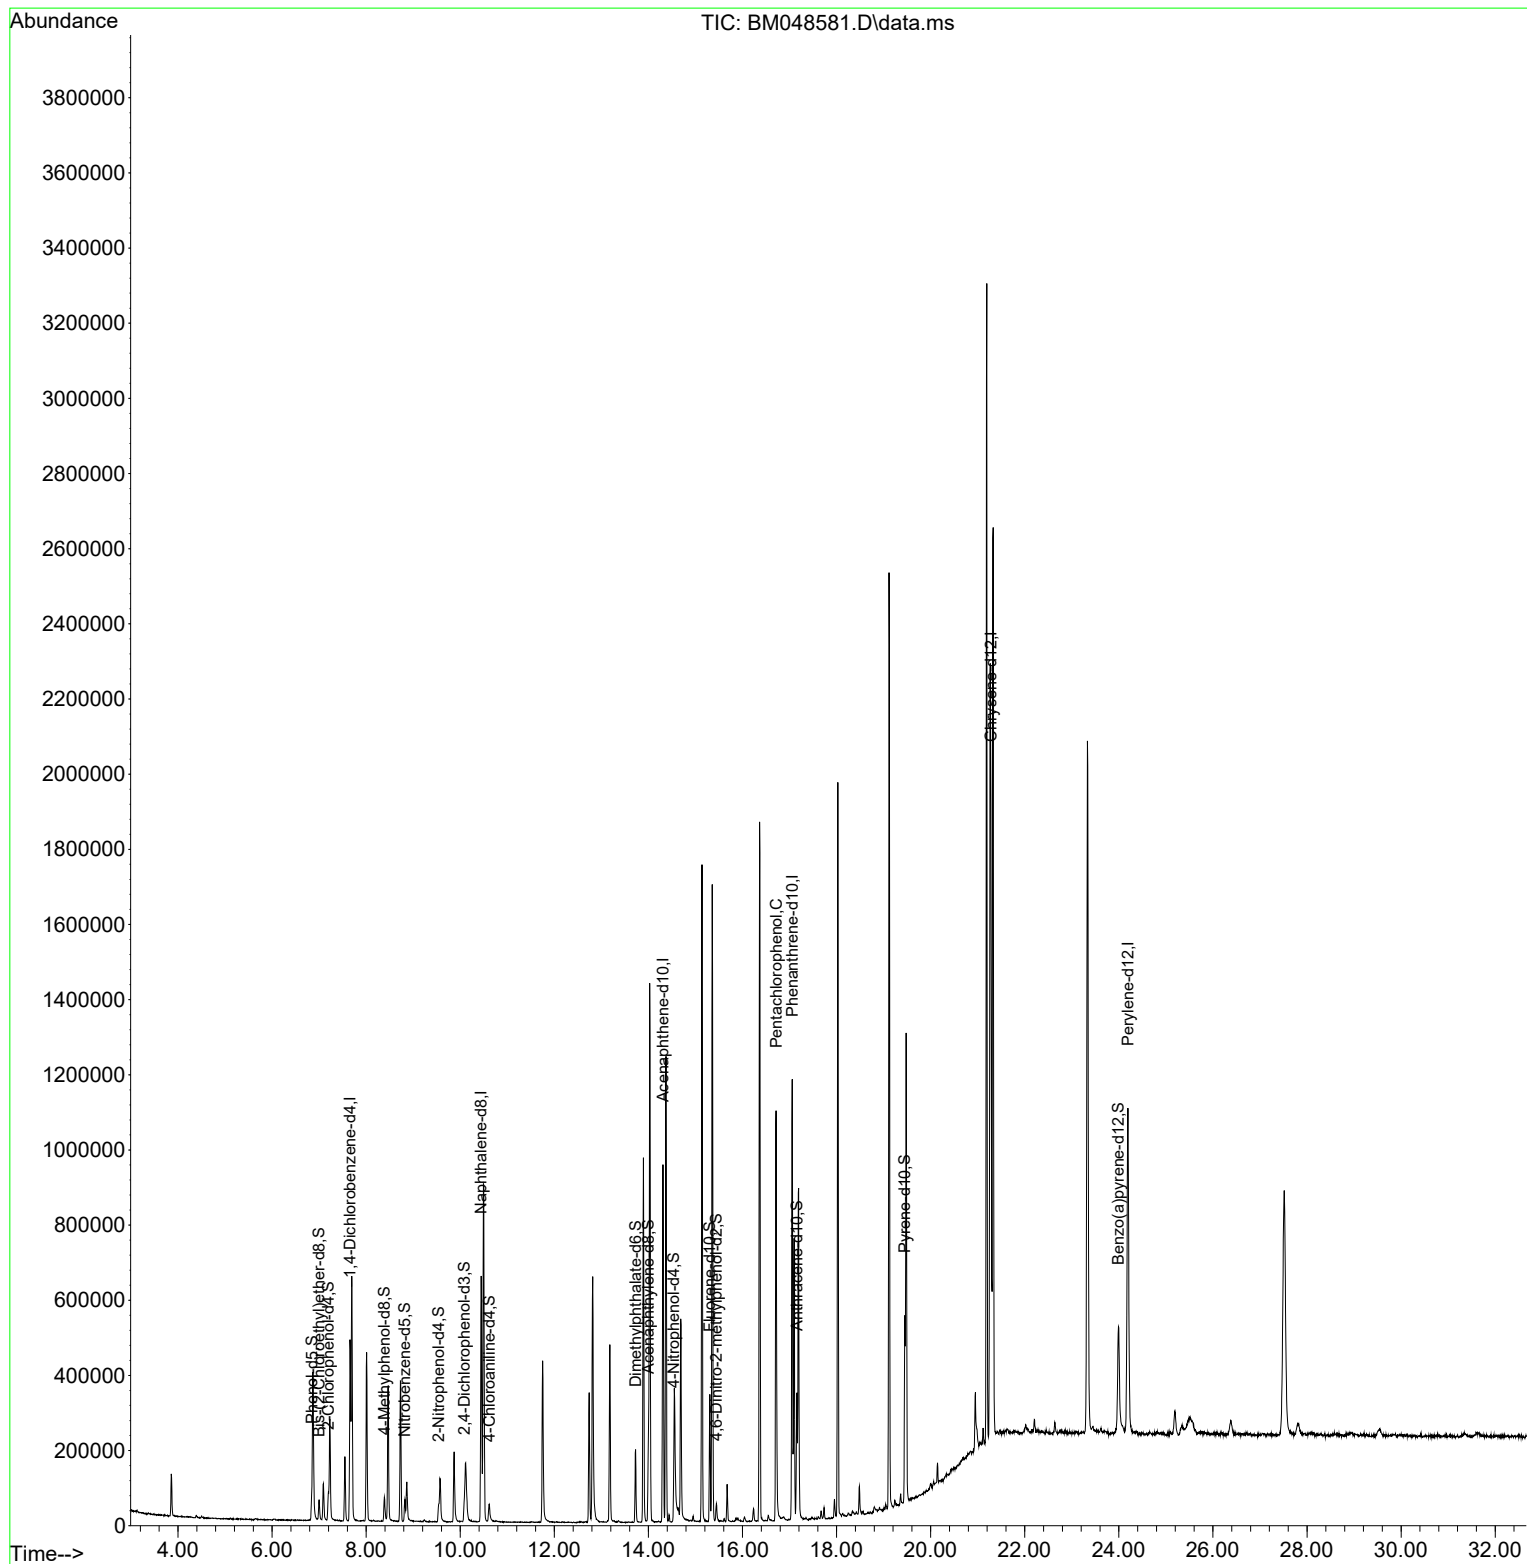

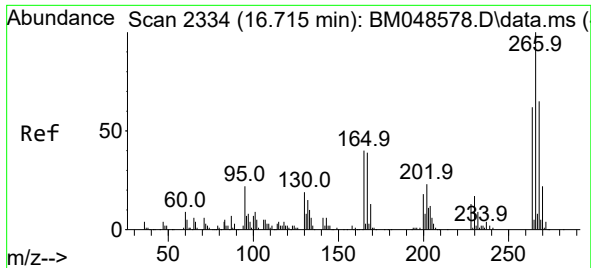

#71
 Pentachlorophenol
 Concen: 41.805 ng/ul
 RT: 16.715 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM048581.D
 Acq: 11 Nov 2024 12:15

Instrument :
 BNA_M
 ClientSampleId :
 GCP54DL

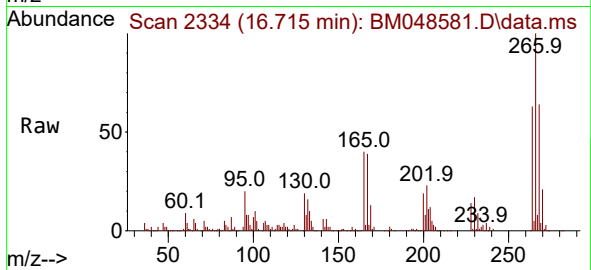

Tgt Ion:266 Resp: 208156
 Ion Ratio Lower Upper
 266 100
 264 62.6 51.1 76.7
 268 63.9 53.2 79.8

