

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048588.D
 Acq On : 11 Nov 2024 17:04
 Operator : RC/JU
 Sample : PB164728BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK728

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	30	rVB	37393	51306	1.60%	0.153%
2	3.540	91	94	119	rBV	442808	755270	23.55%	2.259%
3	3.811	138	140	144	rBV5	3032	3773	0.12%	0.011%
4	3.858	144	148	154	rVB4	8315	13656	0.43%	0.041%
5	5.646	447	452	459	rBV8	3786	9637	0.30%	0.029%
6	5.763	469	472	477	rBV4	1807	3213	0.10%	0.010%
7	6.840	649	655	674	rBV	474659	833146	25.98%	2.492%
8	6.999	675	682	692	rBV	397754	670812	20.91%	2.006%
9	7.193	709	715	727	rBV	524576	877971	27.37%	2.626%
10	7.657	786	794	803	rBV	522540	855231	26.66%	2.558%
11	8.375	909	916	932	rBV	587573	1045842	32.61%	3.128%
12	8.816	982	991	1003	rBV	467109	798534	24.90%	2.388%
13	9.540	1106	1114	1128	rBV	361576	656903	20.48%	1.965%
14	10.081	1199	1206	1233	rBV	522346	1047284	32.65%	3.132%
15	10.446	1260	1268	1280	rBV	746016	1214411	37.86%	3.632%
16	10.593	1286	1293	1314	rBV	414358	961602	29.98%	2.876%
17	12.069	1537	1544	1550	rBV5	6381	14231	0.44%	0.043%
18	13.722	1819	1825	1833	rBV	963493	1412574	44.04%	4.225%
19	13.998	1865	1872	1886	rBV	1214670	1819337	56.72%	5.441%
20	14.310	1918	1925	1934	rBV	1064970	1570701	48.97%	4.698%
21	14.545	1956	1965	1987	rBV	215899	587583	18.32%	1.757%
22	15.304	2087	2094	2109	rBV	1546510	2222075	69.28%	6.646%
23	15.439	2109	2117	2129	rVV	351326	554410	17.29%	1.658%
24	15.551	2132	2136	2140	rVB3	9254	14024	0.44%	0.042%
25	15.863	2185	2189	2193	rBV4	8606	13785	0.43%	0.041%
26	16.410	2279	2282	2287	rBV5	2585	3491	0.11%	0.010%
27	16.545	2300	2305	2307	rBV5	7880	10362	0.32%	0.031%
28	16.592	2312	2313	2318	rVB5	3519	3257	0.10%	0.010%
29	17.051	2385	2391	2402	rBV	1297218	1850100	57.68%	5.533%
30	17.151	2402	2408	2425	rVV	1651094	2496190	77.82%	7.465%
31	17.963	2541	2546	2551	rBV8	4253	8790	0.27%	0.026%
32	18.592	2651	2653	2659	rBV7	3101	4106	0.13%	0.012%
33	19.016	2720	2725	2729	rBV3	21508	30097	0.94%	0.090%
34	19.092	2734	2738	2742	rVV	15508	23933	0.75%	0.072%
35	19.239	2761	2763	2769	rBV7	5801	9675	0.30%	0.029%
36	19.451	2793	2799	2813	rBV	2169374	3049550	95.08%	9.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048588.D
Acq On : 11 Nov 2024 17:04
Operator : RC/JU
Sample : PB164728BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK728

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	20.951	3050	3054	3061	rBV	99721	133687	4.17%	0.400%
38	21.280	3105	3110	3119	rBV	1362939	2107408	65.70%	6.303%
39	23.992	3563	3571	3583	rBV	1364491	3207461	100.00%	9.593%
40	24.192	3597	3605	3620	rVB	956042	2491507	77.68%	7.451%




Sum of corrected areas: 33436925

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048588.D
Acq On : 11 Nov 2024 17:04
Operator : RC/JU
Sample : PB164728BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK728

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

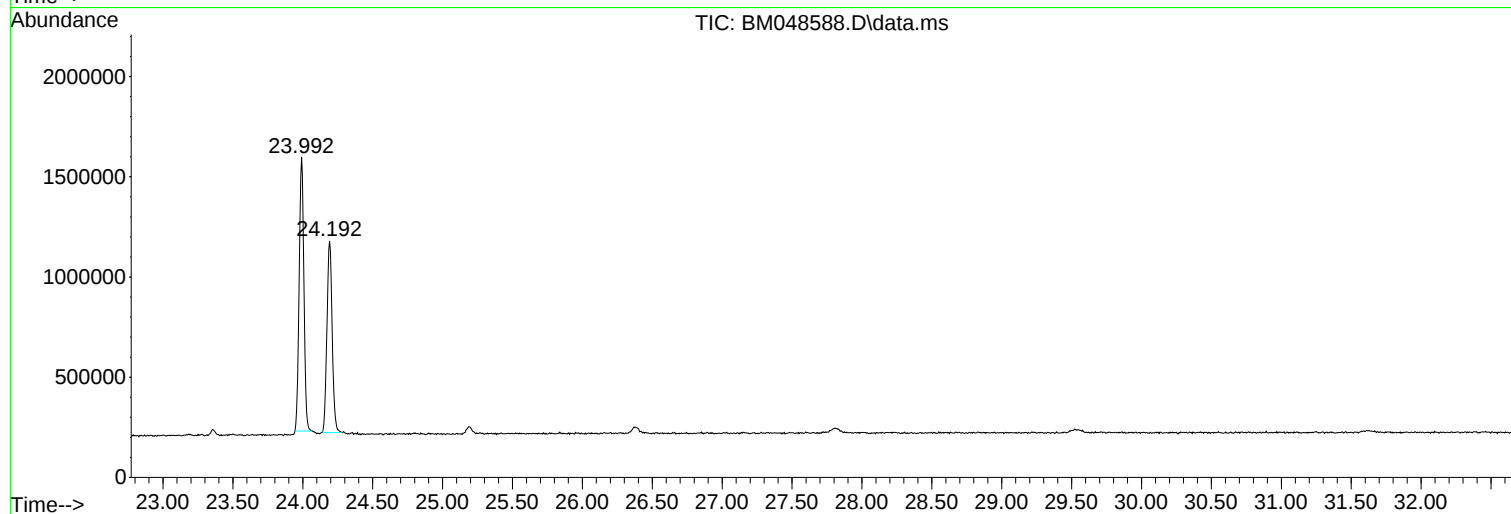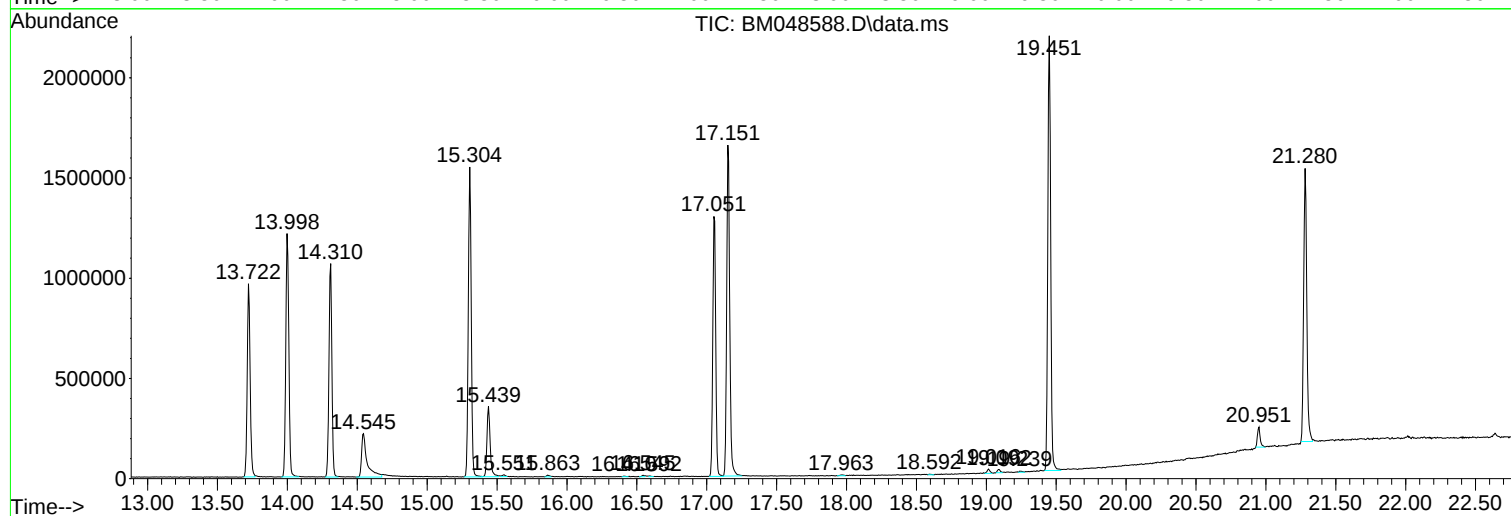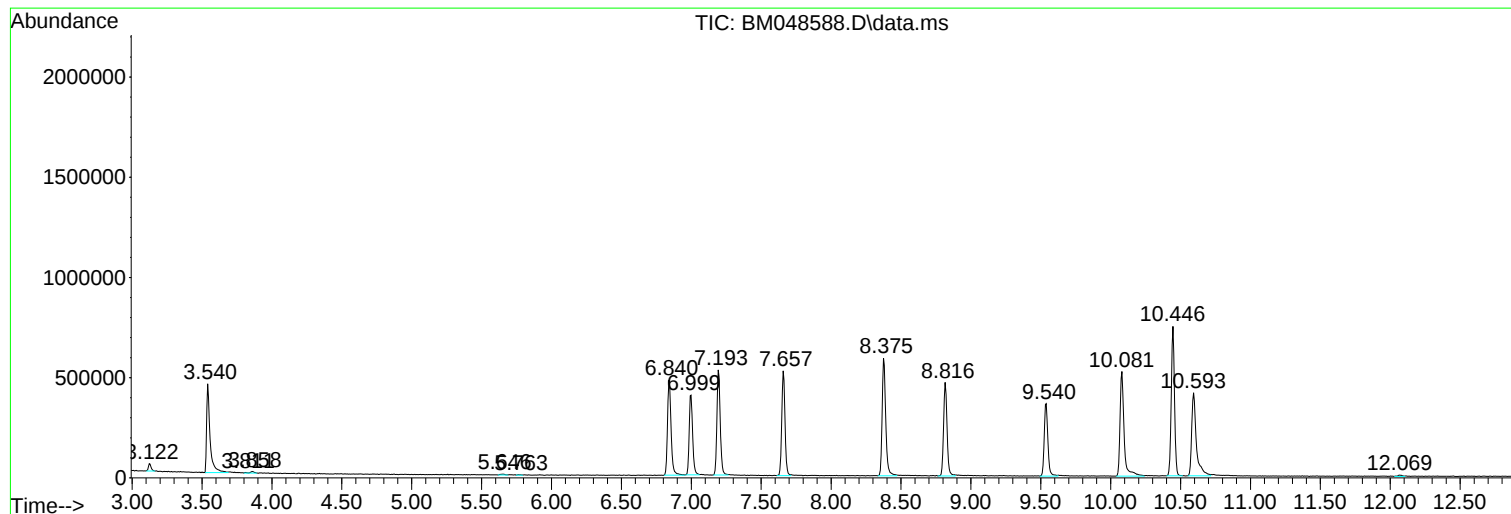

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048588.D
Acq On : 11 Nov 2024 17:04
Operator : RC/JU
Sample : PB164728BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK728

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048588.D
Acq On : 11 Nov 2024 17:04
Operator : RC/JU
Sample : PB164728BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK728

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc