

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048594.D
 Acq On : 11 Nov 2024 21:01
 Operator : RC/JU
 Sample : P4714-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	32	rVB	31514	46301	1.12%	0.130%
2	3.546	92	95	108	rBV	154166	272713	6.58%	0.766%
3	3.857	145	148	152	rBV2	11106	14492	0.35%	0.041%
4	4.369	231	235	242	rBV	19688	30442	0.73%	0.085%
5	5.304	390	394	398	rBV7	3725	6538	0.16%	0.018%
6	5.675	455	457	461	rVB4	7083	8593	0.21%	0.024%
7	5.934	495	501	502	rBV5	4045	5871	0.14%	0.016%
8	6.710	628	633	635	rBV6	3438	4899	0.12%	0.014%
9	6.804	645	649	650	rBV4	3790	5496	0.13%	0.015%
10	6.845	650	656	669	rVB	129172	249087	6.01%	0.699%
11	6.998	675	682	695	rBV	421818	709807	17.13%	1.993%
12	7.193	709	715	725	rBV	485781	829813	20.02%	2.330%
13	7.281	726	730	735	rVB3	17027	26460	0.64%	0.074%
14	7.657	787	794	802	rBV	510767	839792	20.26%	2.358%
15	8.375	909	916	933	rBV	390349	726961	17.54%	2.041%
16	8.816	984	991	1000	rBV	490706	830273	20.03%	2.331%
17	9.534	1106	1113	1123	rBV	382905	684160	16.51%	1.921%
18	10.075	1196	1205	1231	rBV	544261	1111912	26.83%	3.122%
19	10.445	1261	1268	1282	rBV	716531	1211252	29.23%	3.400%
20	10.592	1285	1293	1316	rBV	511630	1159259	27.97%	3.254%
21	12.063	1538	1543	1549	rBV4	6349	13584	0.33%	0.038%
22	12.663	1640	1645	1648	rVB7	2305	4324	0.10%	0.012%
23	13.722	1819	1825	1839	rBV	1150460	1684063	40.64%	4.728%
24	13.998	1865	1872	1888	rBV	1284019	1924200	46.43%	5.402%
25	14.310	1917	1925	1936	rBV	1019451	1554376	37.51%	4.364%
26	14.563	1961	1968	1982	rBV3	39607	140718	3.40%	0.395%
27	15.304	2087	2094	2110	rBV	1816334	2645165	63.83%	7.426%
28	15.439	2110	2117	2133	rVV	452808	716569	17.29%	2.012%
29	15.545	2133	2135	2142	rVB6	11601	18494	0.45%	0.052%
30	15.674	2151	2157	2163	rBV	99412	145956	3.52%	0.410%
31	15.863	2185	2189	2199	rBV8	7672	17025	0.41%	0.048%
32	16.233	2247	2252	2257	rVB7	3850	6633	0.16%	0.019%
33	16.545	2301	2305	2311	rBV6	8607	16613	0.40%	0.047%
34	16.733	2333	2337	2340	rBV5	2763	4426	0.11%	0.012%
35	16.833	2349	2354	2357	rBV6	2816	5805	0.14%	0.016%
36	17.051	2385	2391	2402	rBV	1311366	1852624	44.70%	5.201%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048594.D
 Acq On : 11 Nov 2024 21:01
 Operator : RC/JU
 Sample : P4714-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	17.151	2402	2408	2426	rVV	2169471	3194799	77.09%	8.969%
38	17.268	2426	2428	2435	rVV7	6675	11079	0.27%	0.031%
39	17.345	2437	2441	2448	rVB8	3092	5356	0.13%	0.015%
40	17.886	2530	2533	2537	rBV5	2460	4366	0.11%	0.012%
41	17.951	2537	2544	2550	rBV4	33485	56429	1.36%	0.158%
42	18.721	2673	2675	2677	rBV3	3376	4325	0.10%	0.012%
43	18.792	2685	2687	2690	rBV4	3952	4309	0.10%	0.012%
44	19.015	2721	2725	2730	rVB4	30683	40862	0.99%	0.115%
45	19.086	2733	2737	2742	rBV	28384	37277	0.90%	0.105%
46	19.239	2760	2763	2769	rBV8	13304	20051	0.48%	0.056%
47	19.451	2793	2799	2811	rBV	2798357	3886404	93.78%	10.910%
48	20.945	3050	3053	3066	rBV	101941	181948	4.39%	0.511%
49	21.280	3105	3110	3121	rBV2	1320353	2100989	50.70%	5.898%
50	23.986	3562	3570	3592	rVB	1656753	4144142	100.00%	11.634%
51	24.186	3596	3604	3619	rVB	910914	2403794	58.00%	6.748%




Sum of corrected areas: 35620826

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048594.D
Acq On : 11 Nov 2024 21:01
Operator : RC/JU
Sample : P4714-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

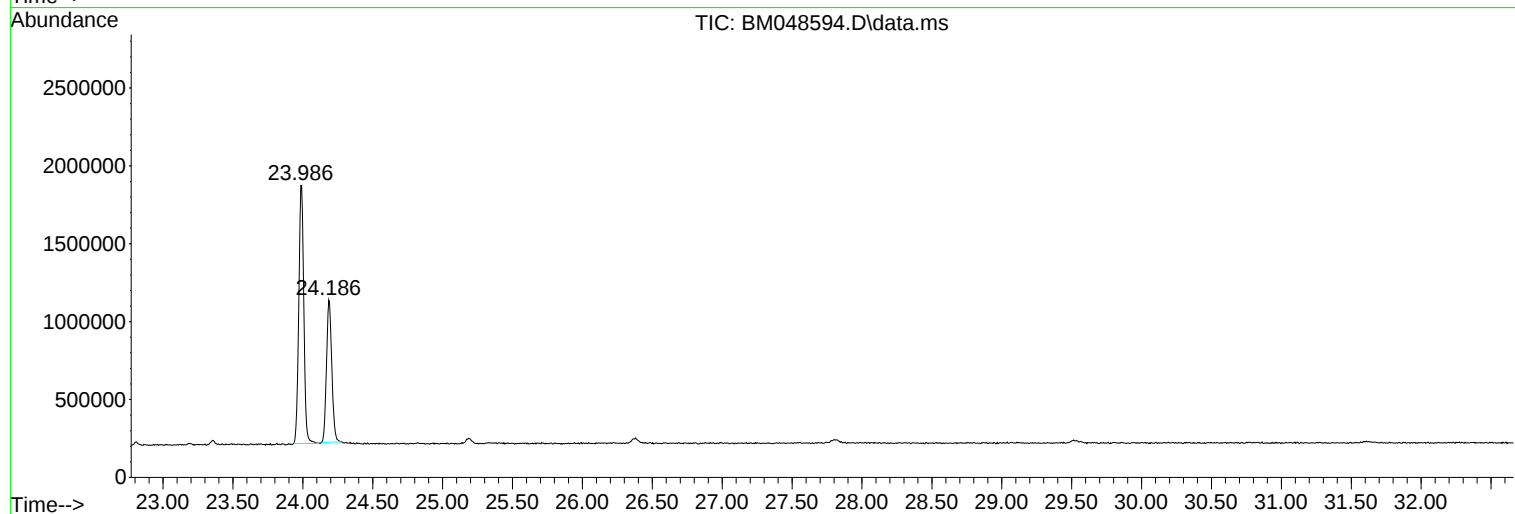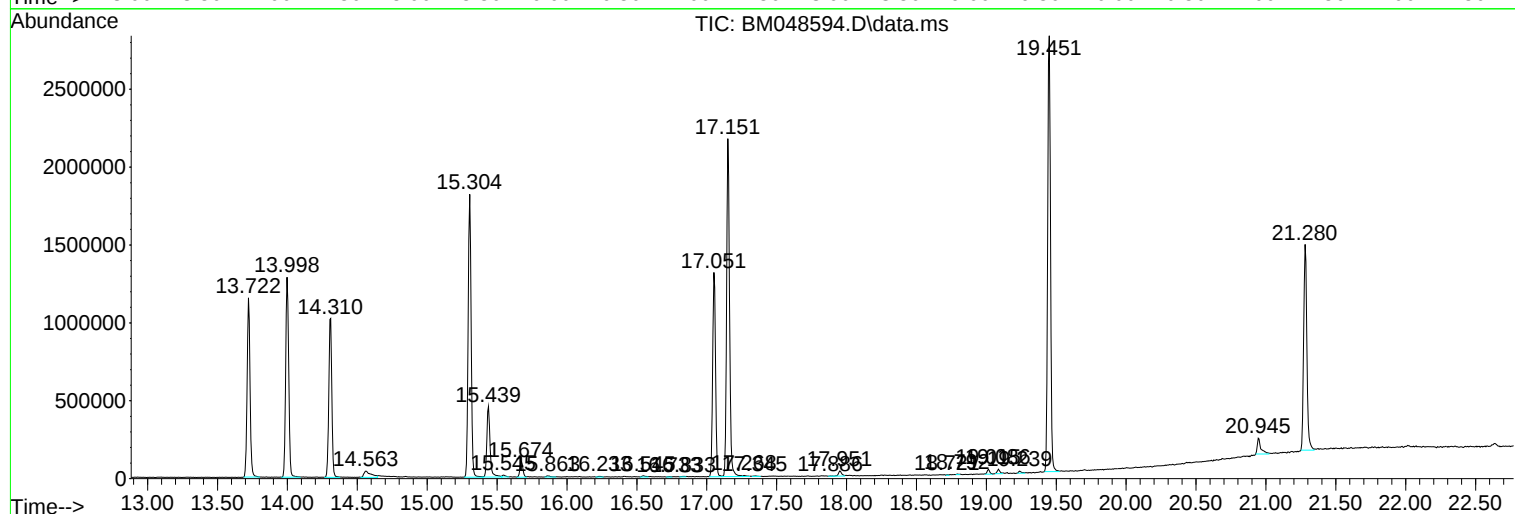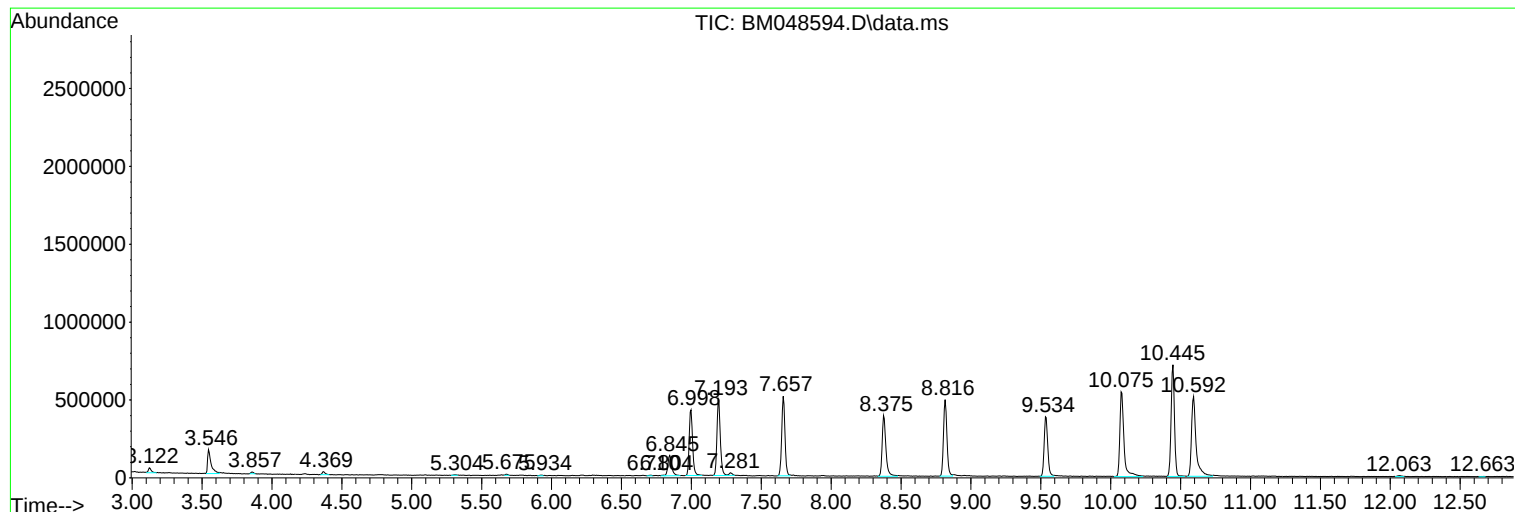

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048594.D
Acq On : 11 Nov 2024 21:01
Operator : RC/JU
Sample : P4714-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048594.D
Acq On : 11 Nov 2024 21:01
Operator : RC/JU
Sample : P4714-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc