

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048596.D
 Acq On : 11 Nov 2024 22:19
 Operator : RC/JU
 Sample : P4714-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	19	23	31	rVB	32294	45939	1.14%	0.126%
2	3.546	92	95	108	rBV	118790	221795	5.50%	0.611%
3	3.858	144	148	154	rVB	37038	51878	1.29%	0.143%
4	4.369	231	235	239	rBV	16412	21836	0.54%	0.060%
5	5.310	391	395	398	rBV5	3435	5622	0.14%	0.015%
6	5.528	426	432	438	rVB8	5392	10171	0.25%	0.028%
7	5.681	455	458	462	rVB5	6676	9416	0.23%	0.026%
8	5.769	469	473	477	rBV6	4707	7228	0.18%	0.020%
9	6.216	545	549	551	rBV5	5378	6909	0.17%	0.019%
10	6.299	560	563	565	rBV3	2918	4232	0.10%	0.012%
11	6.657	620	624	626	rVB3	3448	4162	0.10%	0.011%
12	6.746	637	639	643	rBV4	2879	4314	0.11%	0.012%
13	6.846	650	656	665	rVV	124294	237325	5.88%	0.653%
14	6.993	675	681	694	rBV	423068	719434	17.84%	1.980%
15	7.193	709	715	726	rBV	488176	825978	20.48%	2.274%
16	7.281	726	730	737	rVB2	21612	36458	0.90%	0.100%
17	7.657	787	794	803	rBV	539328	870136	21.58%	2.395%
18	8.375	910	916	932	rBV	400579	733661	18.19%	2.019%
19	8.816	984	991	1000	rBV	497918	830524	20.59%	2.286%
20	8.881	1000	1002	1008	rVB4	9808	14921	0.37%	0.041%
21	9.534	1107	1113	1125	rBV	389652	695387	17.24%	1.914%
22	10.075	1196	1205	1235	rBV	565175	1143572	28.36%	3.148%
23	10.445	1260	1268	1279	rBV	734757	1256458	31.16%	3.459%
24	10.592	1285	1293	1314	rBV	559723	1242104	30.80%	3.419%
25	11.022	1362	1366	1371	rBV6	3403	4629	0.11%	0.013%
26	11.075	1371	1375	1379	rBV5	3784	4980	0.12%	0.014%
27	12.069	1539	1544	1548	rBV2	6526	11088	0.27%	0.031%
28	13.722	1817	1825	1842	rBV	1122258	1688138	41.86%	4.647%
29	13.998	1864	1872	1887	rBV	1333175	1967152	48.78%	5.415%
30	14.304	1918	1924	1933	rBV	1066022	1592851	39.50%	4.385%
31	14.557	1961	1967	1976	rBV3	39273	112228	2.78%	0.309%
32	15.163	2068	2070	2075	rVB5	4075	5700	0.14%	0.016%
33	15.304	2086	2094	2103	rBV	1791338	2642052	65.51%	7.273%
34	15.439	2111	2117	2130	rBV	439853	705716	17.50%	1.943%
35	15.545	2132	2135	2147	rVB9	11724	21926	0.54%	0.060%
36	15.674	2152	2157	2165	rBV	143907	214140	5.31%	0.589%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048596.D
 Acq On : 11 Nov 2024 22:19
 Operator : RC/JU
 Sample : P4714-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	15.863	2185	2189	2195	rBV5	8089	16304	0.40%	0.045%
38	16.198	2241	2246	2249	rBV7	4053	7729	0.19%	0.021%
39	16.239	2249	2253	2258	rVB5	7949	12147	0.30%	0.033%
40	16.480	2291	2294	2297	rBV4	2783	4287	0.11%	0.012%
41	16.545	2301	2305	2313	rVB7	7941	14772	0.37%	0.041%
42	16.821	2349	2352	2353	rBV3	3398	4147	0.10%	0.011%
43	17.051	2385	2391	2402	rBV	1331681	1912373	47.42%	5.264%
44	17.151	2402	2408	2427	rVV	2190310	3197345	79.28%	8.801%
45	17.463	2457	2461	2464	rBV5	3562	5122	0.13%	0.014%
46	17.704	2499	2502	2506	rBV	12529	14952	0.37%	0.041%
47	17.827	2519	2523	2527	rBV6	3886	6594	0.16%	0.018%
48	17.951	2540	2544	2551	rBV2	54295	85678	2.12%	0.236%
49	18.798	2685	2688	2692	rBV6	7927	13053	0.32%	0.036%
50	18.857	2695	2698	2704	rVV5	14458	18472	0.46%	0.051%
51	19.015	2721	2725	2731	rBV	29430	38249	0.95%	0.105%
52	19.086	2733	2737	2741	rBV	28019	43222	1.07%	0.119%
53	19.239	2759	2763	2768	rBV6	22833	38329	0.95%	0.106%
54	19.386	2786	2788	2791	rVB4	7482	5537	0.14%	0.015%
55	19.451	2792	2799	2811	rBV	2734854	3935313	97.58%	10.832%
56	20.945	3050	3053	3065	rBV	100494	184023	4.56%	0.507%
57	21.280	3104	3110	3121	rBV	1434127	2228680	55.26%	6.135%
58	23.991	3562	3571	3584	rVB	1700724	4032828	100.00%	11.101%
59	24.186	3596	3604	3619	rVB	1015424	2539853	62.98%	6.991%




Sum of corrected areas: 36329069

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048596.D
Acq On : 11 Nov 2024 22:19
Operator : RC/JU
Sample : P4714-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

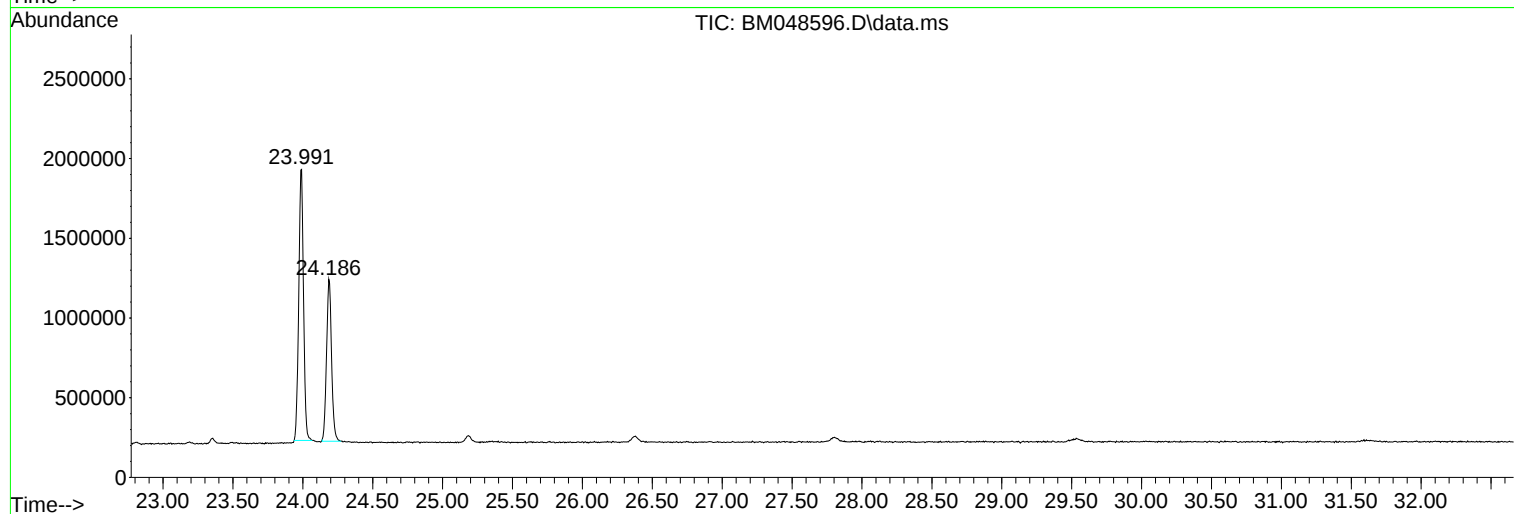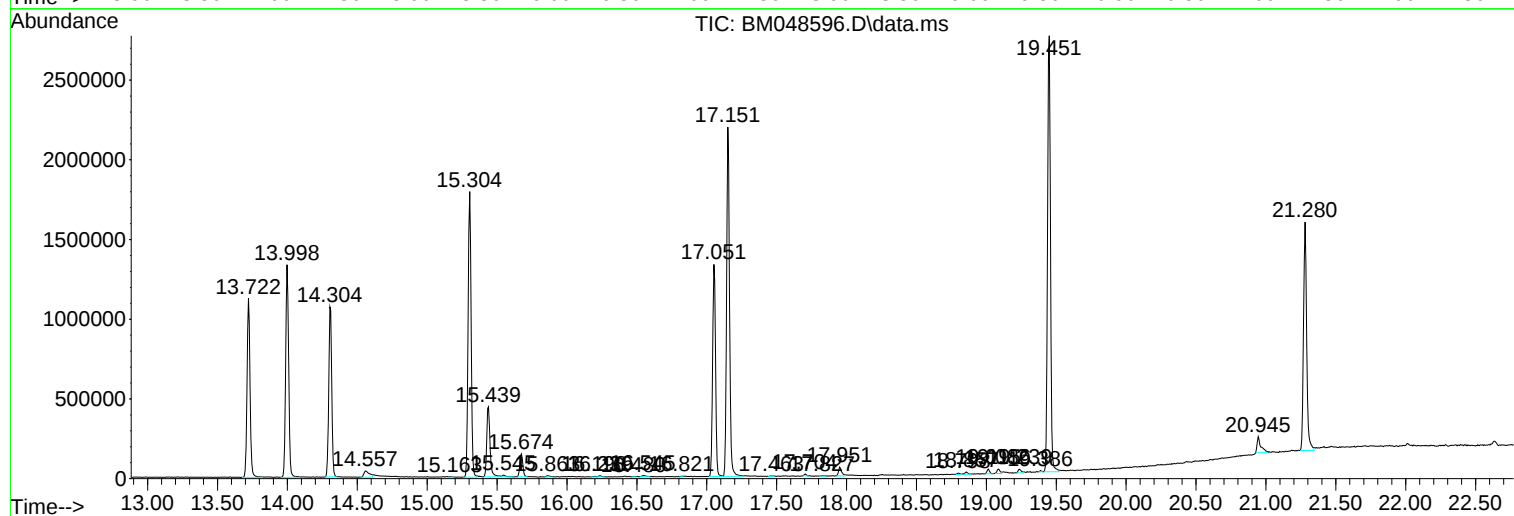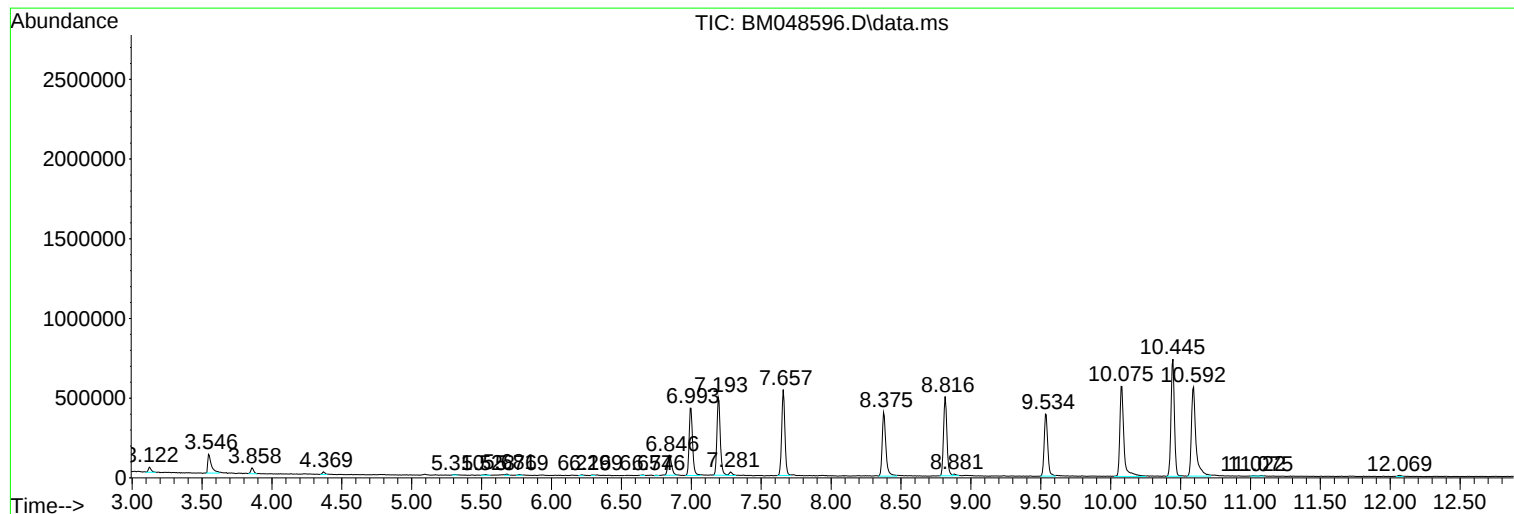

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048596.D
Acq On : 11 Nov 2024 22:19
Operator : RC/JU
Sample : P4714-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.674	2.69 ng/ul	214140	Acenaphthene-d10	14.304

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	95
5			Benzophenone	182	C13H10O	000119-61-9	91

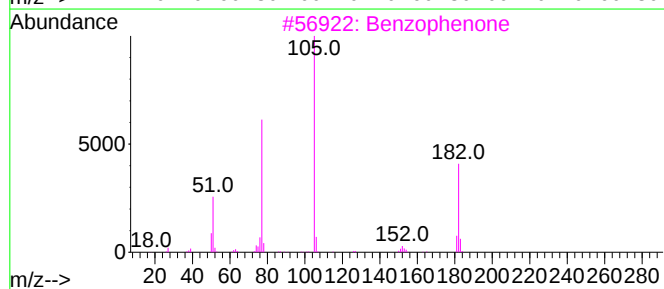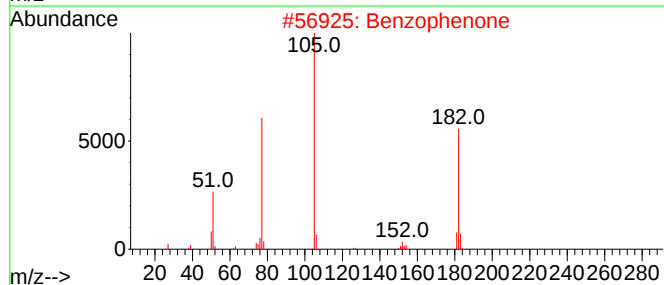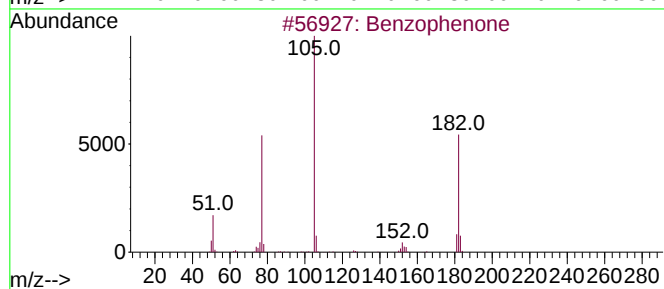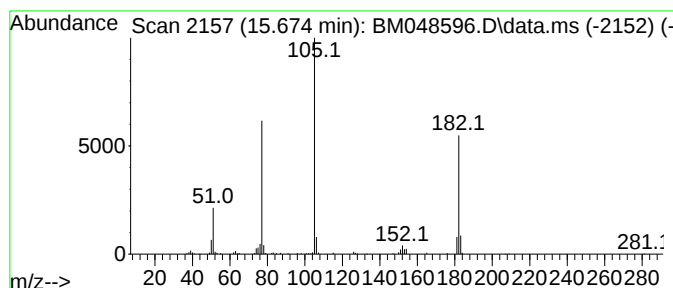

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048596.D
Acq On : 11 Nov 2024 22:19
Operator : RC/JU
Sample : P4714-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.674	2.7	ng/u1	214140	3	14.304	1592850	20.0