

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048598.D
 Acq On : 11 Nov 2024 23:38
 Operator : RC/JU
 Sample : P4668-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	30	rVB	29619	39272	1.04%	0.112%
2	3.552	93	96	107	rBV	67604	129447	3.42%	0.369%
3	3.858	145	148	155	rVB3	9585	16615	0.44%	0.047%
4	4.369	230	235	242	rBV	91580	125738	3.32%	0.359%
5	5.099	355	359	364	rVB7	3379	5959	0.16%	0.017%
6	5.305	391	394	403	rVB6	7937	16774	0.44%	0.048%
7	5.522	426	431	438	rVB	17506	27253	0.72%	0.078%
8	5.652	449	453	454	rBV4	2993	4162	0.11%	0.012%
9	6.322	565	567	573	rBV6	4036	6819	0.18%	0.019%
10	6.846	646	656	673	rVB	138707	279031	7.36%	0.796%
11	6.999	676	682	694	rBV	456335	767177	20.25%	2.189%
12	7.193	708	715	725	rBV	480640	826847	21.82%	2.360%
13	7.346	739	741	747	rVB5	3044	5202	0.14%	0.015%
14	7.475	760	763	767	rBV6	2550	3852	0.10%	0.011%
15	7.657	787	794	804	rBV	532581	862104	22.75%	2.460%
16	8.375	909	916	930	rBV	460643	820977	21.67%	2.343%
17	8.816	984	991	1009	rBV	548228	925692	24.43%	2.642%
18	8.951	1011	1014	1018	rBV5	2869	4315	0.11%	0.012%
19	9.240	1059	1063	1069	rVB5	4906	7400	0.20%	0.021%
20	9.534	1105	1113	1124	rBV	426677	750875	19.82%	2.143%
21	10.075	1198	1205	1230	rBV	541856	1182592	31.21%	3.375%
22	10.445	1259	1268	1277	rBV	728040	1241328	32.76%	3.542%
23	10.598	1286	1294	1310	rBV	207397	547746	14.46%	1.563%
24	12.063	1539	1543	1549	rBV4	7780	13942	0.37%	0.040%
25	12.663	1640	1645	1646	rBV3	3367	4644	0.12%	0.013%
26	12.916	1683	1688	1694	rBV7	3770	6370	0.17%	0.018%
27	13.722	1819	1825	1841	rBV	1200681	1741745	45.97%	4.971%
28	13.998	1864	1872	1883	rBV	1381712	2084706	55.02%	5.949%
29	14.304	1915	1924	1940	rBV	1055017	1610799	42.52%	4.597%
30	14.569	1963	1969	1974	rBV6	19026	46927	1.24%	0.134%
31	15.304	2087	2094	2111	rBV	1801701	2695644	71.15%	7.693%
32	15.439	2111	2117	2129	rVV	427150	664154	17.53%	1.895%
33	15.545	2133	2135	2140	rVB4	10308	14511	0.38%	0.041%
34	15.869	2184	2190	2195	rBV7	6005	12800	0.34%	0.037%
35	16.422	2278	2284	2286	rBV5	3098	4676	0.12%	0.013%
36	16.545	2301	2305	2313	rVV5	7438	13920	0.37%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048598.D
 Acq On : 11 Nov 2024 23:38
 Operator : RC/JU
 Sample : P4668-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

37	16.845	2354	2356	2361	rVB4	3580	4424	0.12%	0.013%
38	17.051	2385	2391	2402	rBV	1362837	1900935	50.17%	5.425%
39	17.151	2402	2408	2423	rVV2	2021504	3029220	79.95%	8.645%
40	17.733	2502	2507	2511	rBV8	2471	4317	0.11%	0.012%
41	17.951	2539	2544	2554	rBV2	96400	157720	4.16%	0.450%
42	19.015	2721	2725	2730	rBV2	27812	36896	0.97%	0.105%
43	19.086	2733	2737	2742	rBV2	24456	41103	1.08%	0.117%
44	19.239	2758	2763	2769	rBV2	93340	144342	3.81%	0.412%
45	19.451	2793	2799	2810	rBV	2582644	3720406	98.20%	10.617%
46	20.945	3050	3053	3061	rVB	96636	125852	3.32%	0.359%
47	21.280	3104	3110	3121	rBV	1385818	2161682	57.06%	6.169%
48	23.986	3562	3570	3583	rVB	1579688	3788758	100.00%	10.812%
49	24.186	3596	3604	3620	rVB	917871	2413664	63.71%	6.888%




Sum of corrected areas: 35041334

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048598.D
Acq On : 11 Nov 2024 23:38
Operator : RC/JU
Sample : P4668-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

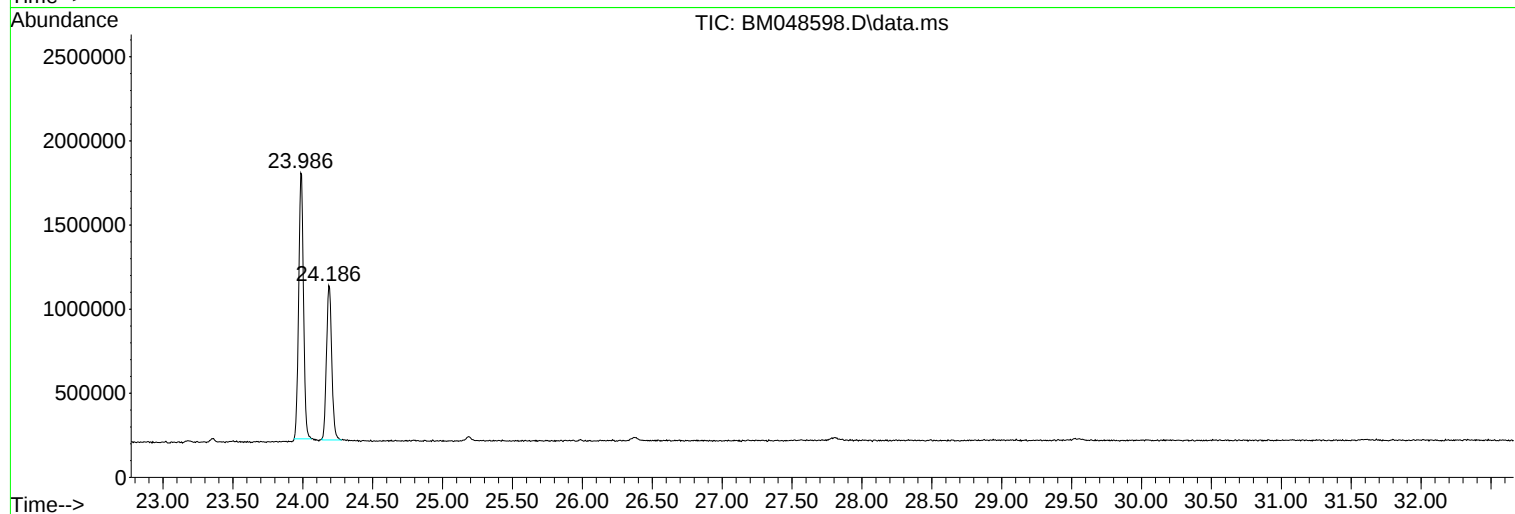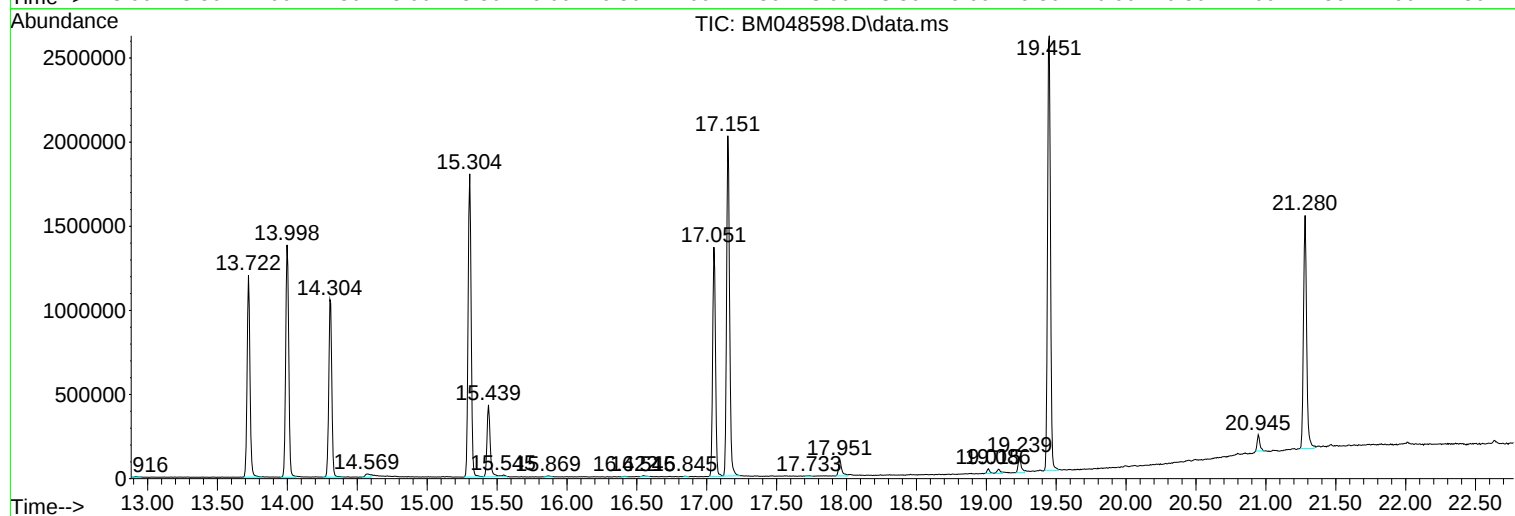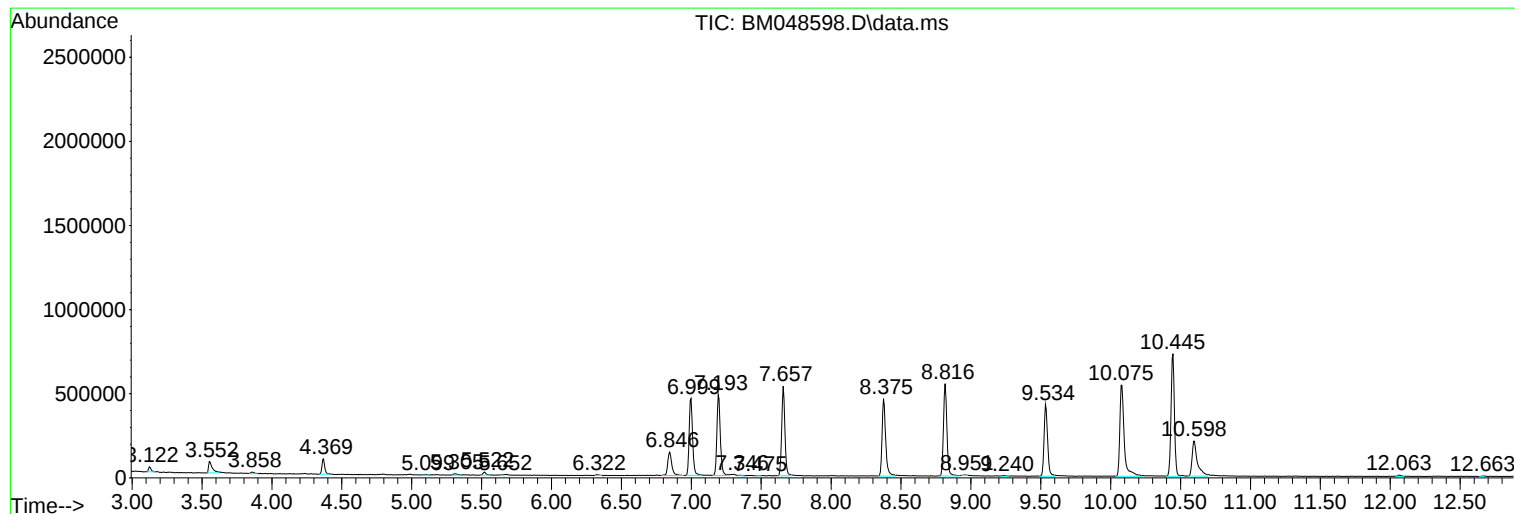

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048598.D
Acq On : 11 Nov 2024 23:38
Operator : RC/JU
Sample : P4668-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048598.D
Acq On : 11 Nov 2024 23:38
Operator : RC/JU
Sample : P4668-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc