

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
 Data File : BM048599.D
 Acq On : 12 Nov 2024 00:18
 Operator : RC/JU
 Sample : P4714-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	31	rVB	37009	52418	1.16%	0.137%
2	3.551	94	96	105	rBV	61656	111049	2.46%	0.291%
3	3.857	146	148	153	rVB4	9699	12719	0.28%	0.033%
4	4.369	231	235	243	rVB	28141	39370	0.87%	0.103%
5	5.304	391	394	397	rBV4	4798	5712	0.13%	0.015%
6	5.675	455	457	464	rVB7	5980	8225	0.18%	0.022%
7	6.222	546	550	554	rVB6	3935	6108	0.14%	0.016%
8	6.292	558	562	567	rBV8	4274	9143	0.20%	0.024%
9	6.704	627	632	635	rBV6	4362	8065	0.18%	0.021%
10	6.845	650	656	668	rVB	124004	232168	5.13%	0.608%
11	6.998	675	682	694	rBV	468153	788332	17.43%	2.063%
12	7.192	709	715	727	rBV	512010	873625	19.32%	2.287%
13	7.281	727	730	739	rVB5	17393	31210	0.69%	0.082%
14	7.369	744	745	751	rVB6	3814	4862	0.11%	0.013%
15	7.481	762	764	773	rVB10	3414	5352	0.12%	0.014%
16	7.657	787	794	805	rBV	563755	908206	20.08%	2.377%
17	7.933	839	841	846	rVB5	3667	4880	0.11%	0.013%
18	8.375	908	916	928	rBV	396648	719944	15.92%	1.884%
19	8.816	984	991	1008	rBV	552465	946200	20.92%	2.477%
20	8.951	1008	1014	1018	rBV4	10867	18278	0.40%	0.048%
21	9.539	1106	1114	1129	rBV	424418	768777	17.00%	2.012%
22	10.080	1198	1206	1217	rBV	596296	1161868	25.69%	3.041%
23	10.445	1261	1268	1283	rVB	777154	1307123	28.90%	3.421%
24	10.592	1286	1293	1313	rBV	315243	754506	16.68%	1.975%
25	11.022	1361	1366	1370	rBV6	2976	5599	0.12%	0.015%
26	11.074	1370	1375	1382	rVV6	2759	6188	0.14%	0.016%
27	12.069	1538	1544	1550	rBV3	7946	16019	0.35%	0.042%
28	13.721	1819	1825	1840	rBV	1334962	1892480	41.84%	4.953%
29	13.998	1865	1872	1884	rBV	1453795	2127456	47.04%	5.568%
30	14.310	1918	1925	1935	rBV	1092028	1672287	36.97%	4.377%
31	14.562	1962	1968	1983	rBV3	37321	131598	2.91%	0.344%
32	14.927	2026	2030	2035	rBV7	6590	8418	0.19%	0.022%
33	15.304	2087	2094	2110	rBV	1948857	2885600	63.80%	7.553%
34	15.433	2110	2116	2132	rVV	538551	873957	19.32%	2.287%
35	15.551	2132	2136	2141	rVB4	10804	17762	0.39%	0.046%
36	15.674	2152	2157	2163	rVB	47576	68030	1.50%	0.178%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048599.D
Acq On : 12 Nov 2024 00:18
Operator : RC/JU
Sample : P4714-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Title : SVOA CALIBRATION

37	15.868	2184	2190	2195	rBV6	8191	16499	0.36%	0.043%
38	15.992	2206	2211	2215	rBV7	8280	13871	0.31%	0.036%
39	16.092	2221	2228	2235	rVB7	4317	9909	0.22%	0.026%
40	16.204	2244	2247	2252	rVB6	3726	6021	0.13%	0.016%
41	16.409	2278	2282	2285	rBV6	3488	4922	0.11%	0.013%
42	16.545	2301	2305	2310	rBV8	7573	11914	0.26%	0.031%
43	16.933	2365	2371	2375	rVB5	5001	8087	0.18%	0.021%
44	17.051	2384	2391	2402	rBV	1386415	2001887	44.26%	5.240%
45	17.151	2402	2408	2430	rVB	2323012	3515987	77.74%	9.203%
46	17.950	2540	2544	2552	rBV3	45730	76469	1.69%	0.200%
47	18.027	2555	2557	2565	rVB8	3863	8787	0.19%	0.023%
48	19.015	2720	2725	2730	rBV2	36429	49194	1.09%	0.129%
49	19.086	2733	2737	2743	rBV	31977	47502	1.05%	0.124%
50	19.239	2759	2763	2767	rBV3	26702	36235	0.80%	0.095%
51	19.386	2786	2788	2792	rVB4	8759	10276	0.23%	0.027%
52	19.450	2792	2799	2809	rBV	3133109	4359473	96.39%	11.410%
53	20.944	3050	3053	3065	rBV	93726	165066	3.65%	0.432%
54	21.280	3104	3110	3122	rBV2	1476979	2290519	50.64%	5.995%
55	23.991	3562	3571	3589	rVB	1887528	4522818	100.00%	11.838%
56	24.185	3596	3604	3616	rVB	1008562	2567101	56.76%	6.719%




Sum of corrected areas: 38206071

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048599.D
Acq On : 12 Nov 2024 00:18
Operator : RC/JU
Sample : P4714-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

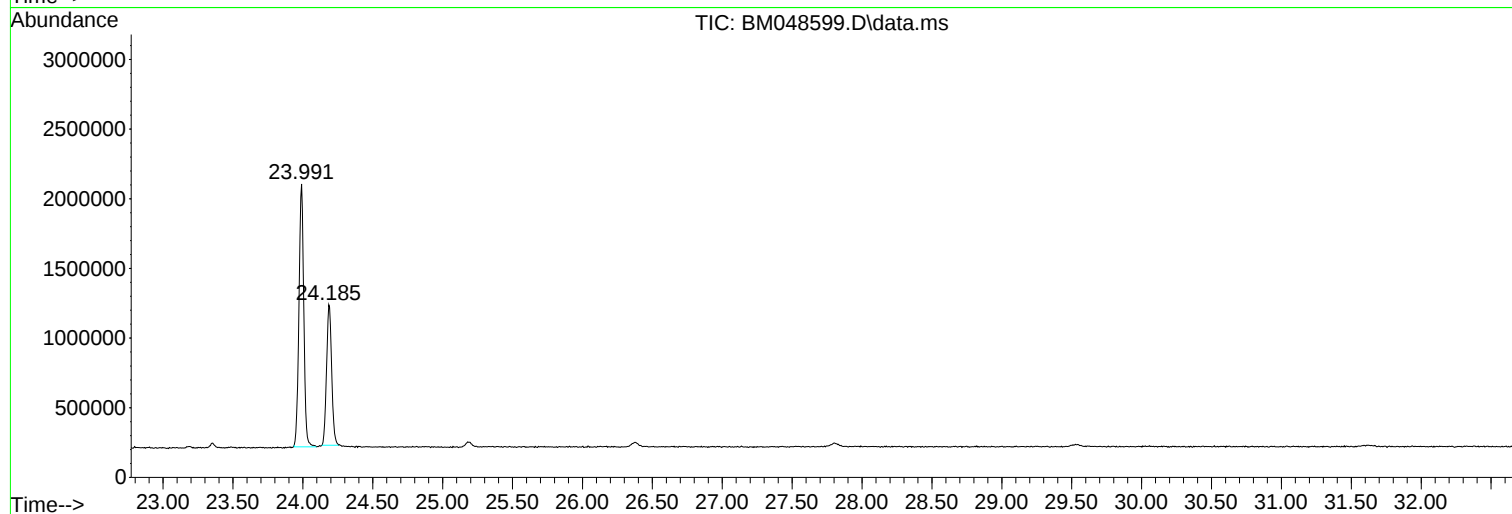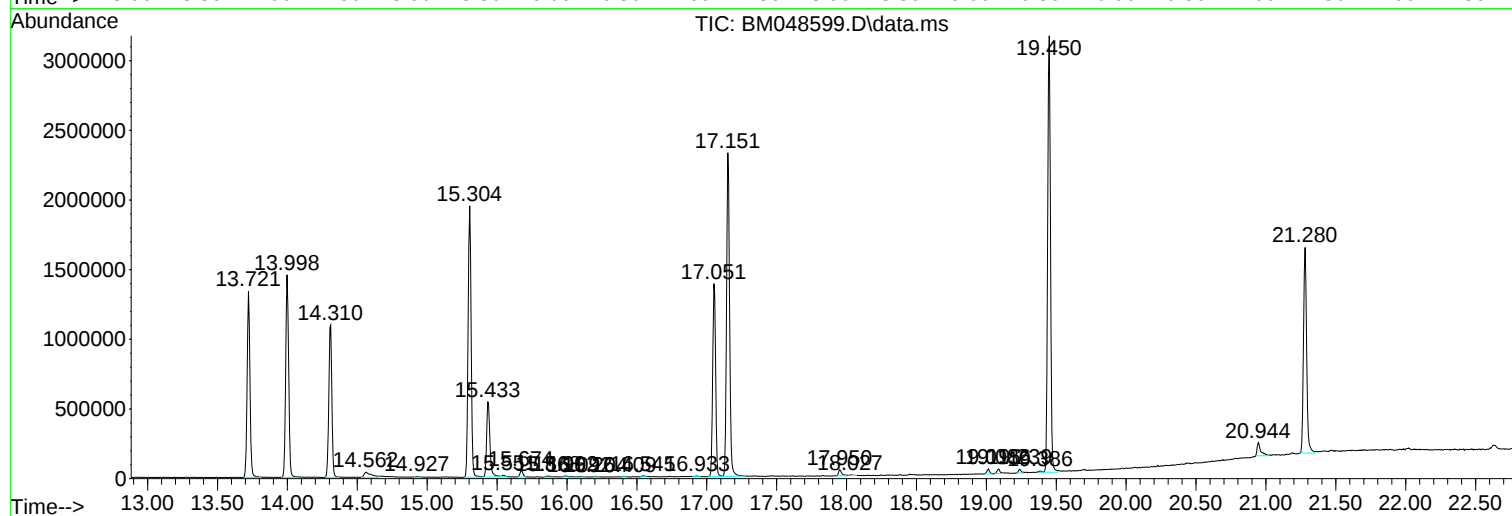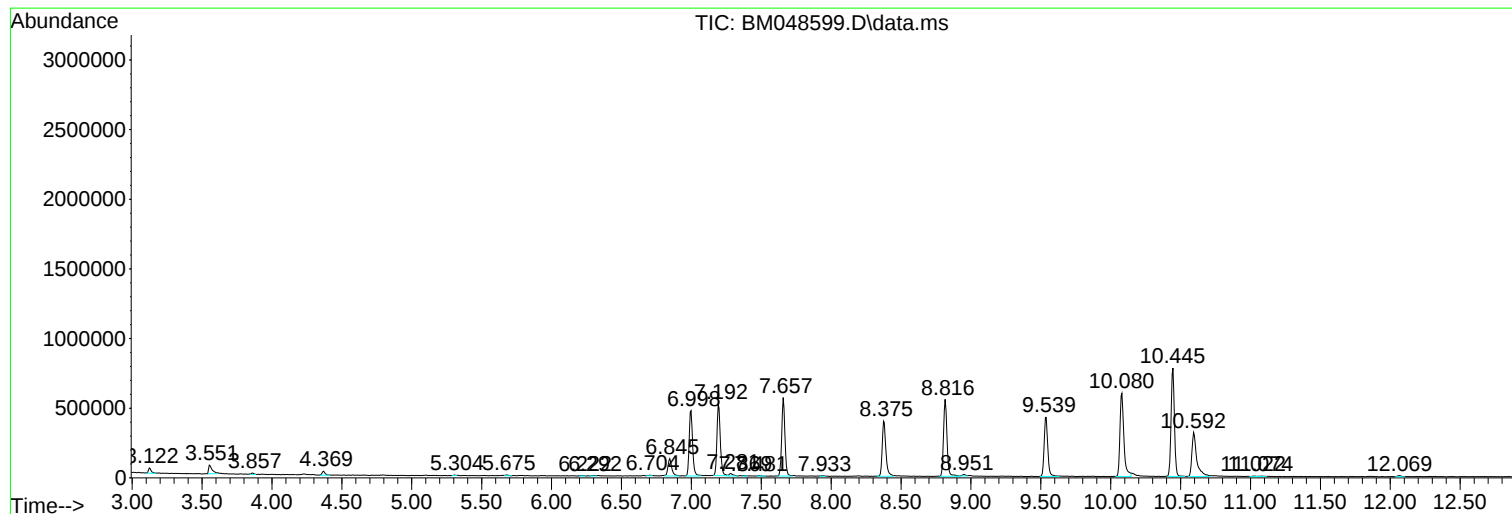

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048599.D
Acq On : 12 Nov 2024 00:18
Operator : RC/JU
Sample : P4714-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111124\
Data File : BM048599.D
Acq On : 12 Nov 2024 00:18
Operator : RC/JU
Sample : P4714-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM110724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc